

Gas analyser

KIGAZ 80



Table of contents

1. Introduction.....	7
1.1. Description of the gas analyser.....	7
1.1.1. Overview of the gas analyser.....	7
1.1.2. Presentation of the keypad and screen.....	8
1.1.3. Connections of the analyser.....	8
1.2. Main features.....	9
1.3. Technical features.....	12
2. Safety.....	13
2.1. Precautions for use.....	13
2.2. Symbols used.....	13
2.3. Safety instructions.....	13
3. Perform a flue gas analysis.....	14
3.1. Prepare the instrument before the analysis.....	14
3.2. Perform an analysis.....	14
3.3. Zoom function.....	15
3.4. Assign the analysis to a customer.....	15
3.5. Add the measurement to a group.....	15
3.6. Print the analysis results.....	15
4. Set the different parameters of the analyser.....	16
4.1. Set the device.....	16
4.1.1. Screen settings.....	16
4.1.2. Set the auto-off.....	16
4.1.3. Change the language.....	16
4.1.4. Modify date and time.....	16
4.1.5. Set the printing of tickets.....	17
4.1.6. Activate or deactivate the visual help.....	17
4.1.7. Activate the group function.....	18
4.1.8. Activate or deactivate Bluetooth® function (optional).....	18
4.1.9. Select the alarm sound.....	18
4.2. Set the combustible.....	18
4.2.1. Modify a combustible.....	18
4.2.2. Add a combustible.....	19
4.2.3. Delete a combustible.....	19
4.3. Set the alarms, measurement units and CO protection.....	19
4.3.1. Set the alarms.....	19
4.3.2. Set the measurement units.....	20
4.3.3. Set the CO protection threshold.....	20
4.3.4. Set the display.....	20
4.4. Set the references.....	20
4.5. Set the duration of auto-zero and purge time.....	20
4.6. Set the operators.....	20
4.6.1. Add an operator.....	21
4.6.2. Modify the operator name.....	21
4.6.3. Delete an operator.....	21
4.7. Back to factory setting of the analyser.....	21
4.7.1. Units and values of measurement settings of the factory setting.....	21
4.7.2. Device factory setting.....	22
5. Manage customers.....	23
5.1. Manage a customer.....	23
5.2. Modify a customer.....	23
5.3. Delete a customer.....	23
6. Manage boilers.....	24
6.1. Create a boiler.....	24
6.2. Modify a boiler.....	24
6.3. Delete a boiler.....	24
7. Manage the inspections.....	25
7.1. Get to inspections.....	25
7.2. Create an inspection.....	25
7.3. Delete an inspection.....	25
7.4. Create a group.....	25

7.5. Add an inspection to a group.....	26
7.6. Delete a group.....	26
8. Perform a control of gas flow.....	27
8.1. Perform a measurement of theoretical flow.....	27
8.2. Perform a measurement of real flow.....	27
8.3. Results interpretation.....	27
9. Perform a gas network leak test.....	28
9.1. Perform the test.....	28
9.2. Link the measurement to a customer.....	28
9.3. Print the results.....	28
10. Perform a pressure measurement.....	29
10.1. Perform the draft measurement.....	29
10.2. Perform a differential pressure measurement.....	29
10.3. Perform a flue gas velocity measurement.....	29
10.4. Link the measurement to a customer.....	29
10.5. Add the measurement to a group.....	30
10.6. Print the results.....	30
11. Perform a measurement of ambient CO ₂	30
11.1. Perform the measurement.....	30
11.2. Link the measurement to a customer.....	30
11.3. Add the measurement to a group.....	30
11.4. Print the results.....	30
12. Perform a measurement of Max CO.....	31
12.1. Perform the measurement.....	31
12.2. Link the measurement to a customer.....	31
12.3. Add the measurement to a group.....	31
12.4. Print the results.....	31
13. Perform some temperature measurements.....	32
13.1. Perform a measurement of ambient temperature.....	32
13.2. Perform a measurement of flue gas temperature.....	32
13.3. Perform an ambient temperature measurement with the internal sensor.....	32
13.4. Perform a Flow/Return temperature measurement.....	32
13.5. Link the measurement to a customer.....	32
13.6. Add the measurement to a group.....	33
13.7. Print the results.....	33
14. Perform a measurement of opacity.....	34
14.1. Perform the measurement.....	34
14.2. Enter the indexes in the analyser.....	34
14.3. Link the measurement to a customer.....	34
14.4. Add the measurement to a group.....	34
14.5. Print the results.....	34
15. Perform a measurement of ionisation current.....	35
15.1. Perform the measurement.....	35
15.2. Link the measurement to a customer.....	35
15.3. Add the measurement to a group.....	35
15.4. Print the results.....	35
16. Perform a flue gas velocity measurement with a Pitot tube.....	36
16.1. Link the measurement to a customer.....	36
16.2. Add the measurement to a group.....	36
16.3. Print the results.....	36
17. To get to information about the analyser.....	37
18. Maintenance of the analyser.....	38
18.1. Life-time of the sensors.....	38
18.2. Replace the sensors.....	38
18.3. Replace the battery.....	39
19. Calculations of the different parameters.....	40
19.1. CO conversion.....	40
19.2. Calculation of flue gas velocity.....	40

1. Introduction.....	42
2. Software installation.....	42
2.1. Recommended minimum configuration.....	42
2.2. Installation.....	42
3. Start with the software.....	43
3.1. Meaning and functions of the menus bar (1).....	43
3.2. Meaning and functions of tool bar buttons (2).....	44
3.3. Meaning and functions of the homepage buttons (3).....	44
4. Download inspections.....	44
5. Use the different databases.....	45
5.1. Use the customer database.....	45
5.2. Use the boilers database.....	46
5.3. Complete database.....	48
5.3.1. Database settings.....	48
5.3.2. Save while using.....	48
5.3.3. Import a database.....	48
5.4. Edit an analysis report.....	49
6. Set the analyser.....	50
6.1. Change the combustibles.....	50
6.2. Change the references.....	50
6.3. Manage the operators.....	50
6.4. Modify the date and time.....	51
6.5. Sensors state.....	51
6.6. Set printings.....	51
6.7. Battery level.....	51
6.8. Access to information about the instrument and update the instrument.....	51
6.8.1. Access to information about the instrument.....	51
6.8.2. Update the device.....	51
The Internet connection is not protected by a proxy.....	51
The Internet connection is protected by a proxy.....	52
6.8.3. Install a 3 rd language.....	52
6.8.4. Send a report of the device to the After-Sales Service.....	53
6.8.5. Back to factory parameters.....	53
7. Options.....	53
7.1. E-mail.....	53
7.2. User information.....	53
7.3. Change the language.....	53
8. Customers / Boilers deletion of the analyser.....	54
9. Compare the instrument and software information.....	55
9.1. Add elements automatically in the databases.....	55
9.2. Modification of customer and boilers features.....	55

1. Introduction

1.1. Description of the gas analyser

The KIGAZ 80 is a gas analyser with **two interchangeable sensors (O₂ and CO-H₂)**.

Its main features are the following:


- Sensors protection by pump stopping and configurable thresholds
- Users management
- Creation and edition of inspections with the external printer as option
- 15 programmed combustibles and possibility to add up to 5
- 2 GO of memory

The gas analyser is supplied in a transport case with a magnetic protective cover, a flue gas probe and its water trap, a Li-Ion battery and its charger, the LIGAZ-2 software which allows inspection creation, a USB cable and a calibration certificate.



This analyser is designed to control parameters of flue gas in exhaust duct or heating units. It can not be used in a permanently way and/or used as an alarm system.


1.1.1. Overview of the gas analyser

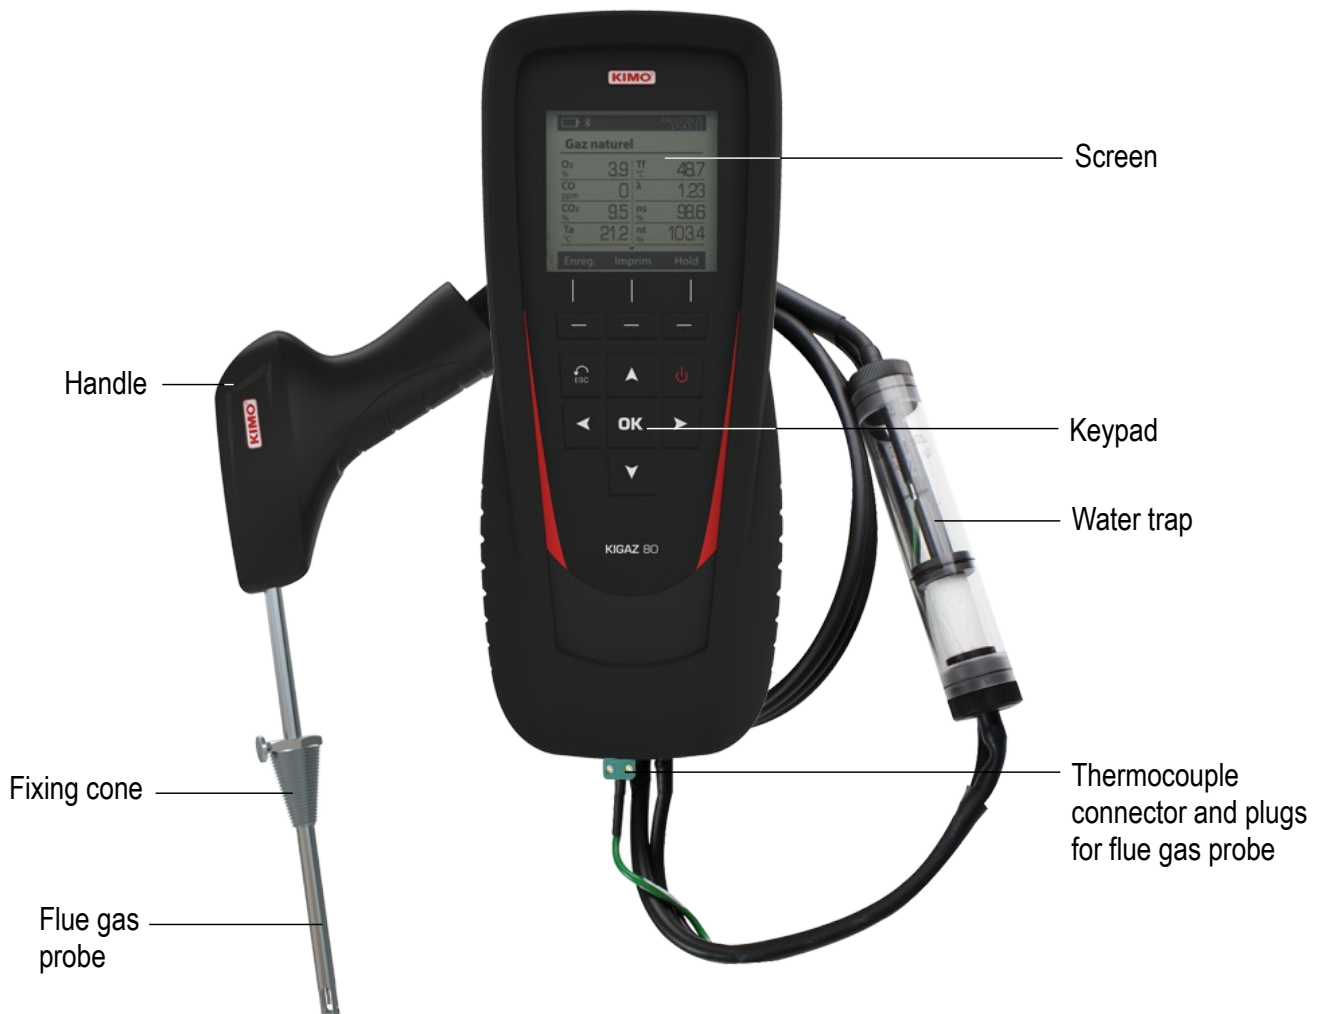

1.1.2. Presentation of the keypad and screen



1.1.3. Connections of the analyser

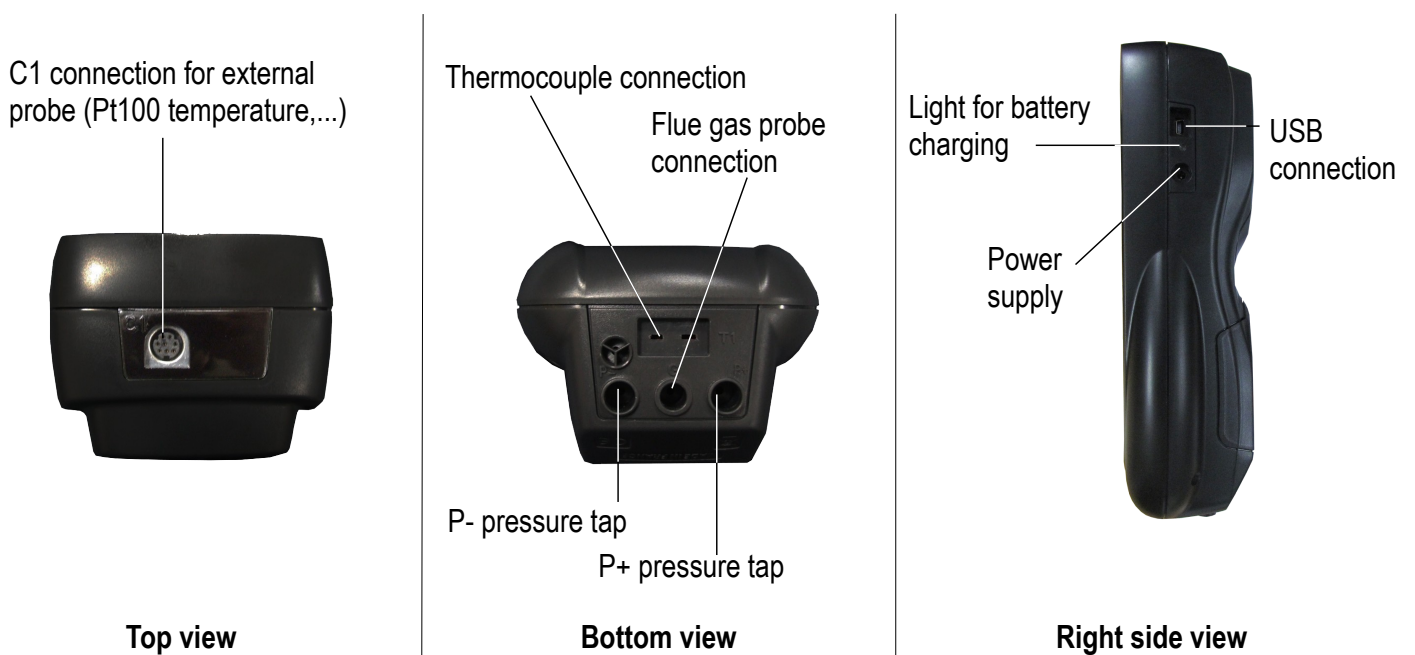

1.2. Main features

- **Screen**

Graphic grey-scales back lighted screen, 54 x 50 mm. It allows to display the measured parameters in a comfortable format for the user. With the zoom function, the measured values can be visualized in increased characters.

- **Printer**

The printer has 10-year guarantee thermal paper. The printer has an easy replacement system of the paper (Easyload). In addition, printing is fast.

- **Batteries charger**

The instrument is supplied with a 6 V, 1.5 A power adapter to load the internal batteries. The current loading is indicated by a battery symbol on the top left of the screen. The red LED on the right side of the gas analyser stays on until the battery loading is completed. The power supply voltage is 100-240 VAC, 50/60 Hz. The battery charging time is 10 hours. The number of cycles of the battery is about 500 charging cycles.

- **Flue gas suction pump**

The pump, inside the gas analyser, is a diaphragm pump with a motor. It is energized in direct current directly by the instrument in a way to get an optimal suction of flue gases.

- **Flue gas probe**

Probe in stainless steel with an over-moulded handle in plastic, with a standard length of 15 cm with a fixing cone to maintain the contact tip in the duct. Interchangeable, it is connected to the instrument by a neoprene tube of 2.50 m.

- **Measurement sensors**

The analyser uses electrochemical sensors to measure the oxygen and the carbon monoxide (compensated in H₂ hydrogen).

- **Temperature sensors**

Flue gas temperature is measured with a thermocouple integrated in the contact tip. The connection to the analyser is made thanks to a single male connector compensated in temperature. K thermocouple (nickel-nickel chromium) allows continuous measurements up to **1250 °C**.

The instrument has a NTC thermoresistance for the measurement of internal temperature; this sensor is also used for the measurement of ambient temperature.

If a temperature control of the combustive air must be performed directly by the supply duct (room sealed boiler), a Pt100 temperature probe (ref: SPA 150 SP) will be used. It is recommended to perform this measurement to make the efficiency calculation of the installation more accurately.

- **Supply input of flue gases and +/- pressure**

The analyser has 3 connectors: Pressure +, Pressure - and Gas. They have a mistake-proofing system for an easy connection.

- **Types of combustibles**

The analyser is supplied with a memorisation of technical data which characterises the 15 most known combustibles. It is also possible to add 5 combustibles and their corresponding features.

- **Calibration certificate**

The analyser is calibrated by comparison with standard of metrology laboratories, which are periodically certified closed to laboratories known at the international level. Each analyser is supplied with its calibration certificate in which, for every parameters, are indicated the nominal value, the one measured, the admitted error limits and the found error.

- **Conformity and standards**

The analyser complies with n°2004/108/EC directive on electromagnetic compatibility. Document available on request. It also complies with 2006/95/EC Low Voltage, 2011/65/EU RoHS II and 2012/19/WEE directives. Moreover, the analyser complies with EN 50379-1 and 50379-2 standards.

- **Water trap**

The water trap is placed on the tube that links the flue gas probe to the Kigaz 80. The measured gases go through the filtering element allowing the recovery of condensates (liquid or solid one).


The filtering element is placed 15 cm from the analyser and is divided into 2 parts:

- one recovers the liquid particles,
- the other contains a filter that stops the smallest particles in suspension and avoid them to reach the electro-chemical sensors.

Condensates are evacuated by opening the plug.



For a better measurement, the water trap must be in vertical position. Empty and clean the water trap after use.

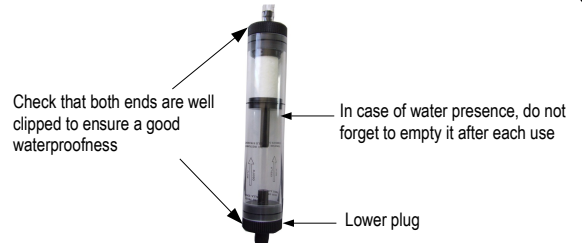

The presence of a water trap with filter can cause some gases solubility in water during gas analysis.

- **Auto-zero**

The analyser has the auto-zero function: it allows to suck ambient and set the sensors to 0 ppm.

- **CO protection**

The analyser is equipped with the CO protection function that allows to avoid high concentrations of CO that could damage the analyser and the sensors. The suction-pump is stopped when it exceeds a threshold defined by the user. However, during a flue gas analysis, it is possible to stop the pump manually at any time by pressing the **OK** button.

- **Customers, boilers and inspections management**

The analyser allows to record customers, theirs respective boilers and inspections. Once the features of customers and boilers are completed in the analyser, the operator can easily assign the different measured values to a customer and his boiler.

- **Opacity index measurement (optional)**

It is possible to fill in the analyser with opacity index values measured according to the Bacharach scale. The analyser will calculate the average and results will be printed on the ticket. This measurement must be performed with an opacity pump which is available as an accessory (ref: PMO).

- **Gas network leak testing (optional)**

It is possible to check the tightness of an installation. For this control, use the pressure sensor used for the differential pressure measurement of the shaft.

- **Measured values**

- **O₂**: percentage of oxygen in flue gases
- **CO**: concentration of CO in flue gases
- **T_f**: flue gases temperature
- **T_a**: combustive air temperature

- **Calculated values**

- **λ: Air Excess** : connection between the volume of combustive air and the requested volume necessary for a combustion in stoichiometric conditions.
- **CO₂**: percentage of carbon dioxide in flue gases.
- **ΔT**: difference between the flue gases temperature and the combustive air temperature.
- **Qs**: percentage of waste heat throughout the chimney
- **ηs: Lower efficiency (or sensible)**: calculated burner efficiency. This is a ratio between the conventional heating

power end the burner heating power. Among the combustion losses, only the sensible heat lost with the flue gases is taken into account, neglecting the radiation losses and incomplete combustion losses. This value is referred to LHV (Lower Heating Value) and can not be higher than 100%.

The sensible efficiency value is to be compared with the minimum efficiency stated for the heating systems performances.

- **η_t : Higher efficiency (or total):** is the sum of sensible efficiency and the additional efficiency deriving from the recovery of water vapour condensation contained in the flue gases. When it is greater than sensible efficiency, then condensation is taking place. It is referred to LHV (Lower Heating Value) and can exceed 100%. The LHV is calculated by an algorithm developed by Kimo and its value must be considered as indicative.

- **CO (O₂):** Concentration of CO in flue gases in mg/m³. It is calculated according to O₂ reference value indicated in the analyser (see page 20).

1.3. Technical features

Parameter	Sensor	Measuring range	Resolution	Accuracy*	T ₉₀ response time
O ₂	Electro-chemical	From 0 % to 21 %	0.1 % vol.	±0.2 % vol.	30 s
CO (with H ₂ compensation)	Electro-chemical	From 0 to 8000 ppm	1 ppm	From 0 to 200 ppm: ±10 ppm From 201 to 2000 ppm: ±5 % of measured value From 2001 to 8000 ppm: ±10 % of measured value	30 s
Flue gas temperature	K thermocouple	From -100 to +1250 °C	0.1 °C	±0.4% of measured value or ±1.1 °C	45 s
Ambient temperature	Internal NTC	From -20 to +120 °C	0.1 °C	±0.5 °C	
Ambient temperature	Pt100 (1/3 DIN external probe)	From -50 to +250 °C	0.1 °C	±0.3 % of measured value ±0.25 °C	30 s
Dew-point temperature	Calculated**	From 0 to +99 °Ctd	0.1 °C	-	-
DHW temperature	TcK (external probe)	From -200 to +1300 °C	0.1 °C	±0.4 % of measured value ±1.1 °C	-
Differential pressure	Semiconductor	From -20 000 to +20 000 Pa	1 Pa	From -20 000 to -751 Pa: ±0.5 % of measured value ±4.5 Pa From -750 to -61 Pa: ±0.9 % of measured value ±1.5 Pa	-
Draft		From -10 to +10 Pa From -1000 to +1000 Pa	0.1 Pa 1 Pa	From -60 to 60 Pa: ±2 Pa From 61 to 750 Pa: ±0.9 % of measured value ±1.5 Pa From 751 to 20 000 Pa: ±0.5 % of measured value ±4.5 Pa	
Losses	Calculated**	From 0 to 100 %	0.1 %	-	-
Excess air (λ)	Calculated**	From 1 to 9.99	0.01	-	-
Lower efficiency (η _s)	Calculated**	From 0 to 100 %	0.1 %	-	-
Higher efficiency (η _t) (condensing)	Calculated**	From 0 to 120 %	0.1 %	-	-
Opacity index	External instrument	From 0 to 9	-	-	-

* All accuracies indicated in this document were stated in laboratory conditions and can be guaranteed for measurements carried out in the same conditions, or carried out with required compensation.

** Calculation is made based on the measured values by the analyser.

2.1. Precautions for use

Please always use the device in accordance with its intended use and within parameters described in the technical features in order not to compromise the protection ensured by the device.

2.2. Symbols used

For your safety and in order to avoid any damage of the device, please follow the procedure described in this user manual and read carefully the notes preceded by the following symbol:



The following symbol will also be used in this user manual:

Please read carefully the information notes indicated after this symbol.



2.3. Safety instructions



**The following safety instructions have to be strictly observed.
Not respecting these safety instructions can lead to a loss of warranty.**



- The analyser should not to be used in and under water.
- The analyser should not to be placed near or directly at open fire or heat.
- The indicated range of temperature of the probe is not to be exceeded, as the probe and temperature sensor could be destroyed.
- After measurements, before packing the analyser, wait for the probe to be cold. As long as it is hot, the probe could produce injuries.
- The exhalations of alcohol liquids (lubricants, petrol, spirit, vanish...) may damage the sensors of the analyser. Therefore, it is forbidden to preserve or use these fluids nearby the analyser.
- Load the battery only with Kimo charger. The charger must be used only for the power supply loading. Use another type of charger can damage the battery and the analyser and can cause electrical shocks.


3. Perform a flue gas analysis

3.1. Prepare the instrument before the analysis

 During the measurement, the analyser must be in vertical position or in horizontal position. Do not hold the analyser in inclined position.



 Before the 1st use of the analyser, a full charge of the battery must be made during 12 hours.

 Empty the water trap.

 In case of any default or damage of the instrument, Kimo After sales service shall be contacted. On the back of the analyser, there is a label with the analyser serial number. This number shall be communicated for every operation (technical operation or request of spare parts).

3.2. Perform an analysis

- Connect the flue gas probe to the analyser.
- Turn on the instrument.
Home screen is displayed with measurement menu highlighted.
- Press **OK**.
Remaining time of autozero and its progress bar are displayed at the bottom of the screen. The screen with the different possible measurements is displayed.
- Go to **“Combustion”** with up and down arrows.
- Press **OK**.
The screen displays the different combustibles in the analyser.
- Select the type of used combustible by the boiler with with up and down arrows.
- Press **OK**.
The screen displays values of the different parameters of the analysis.

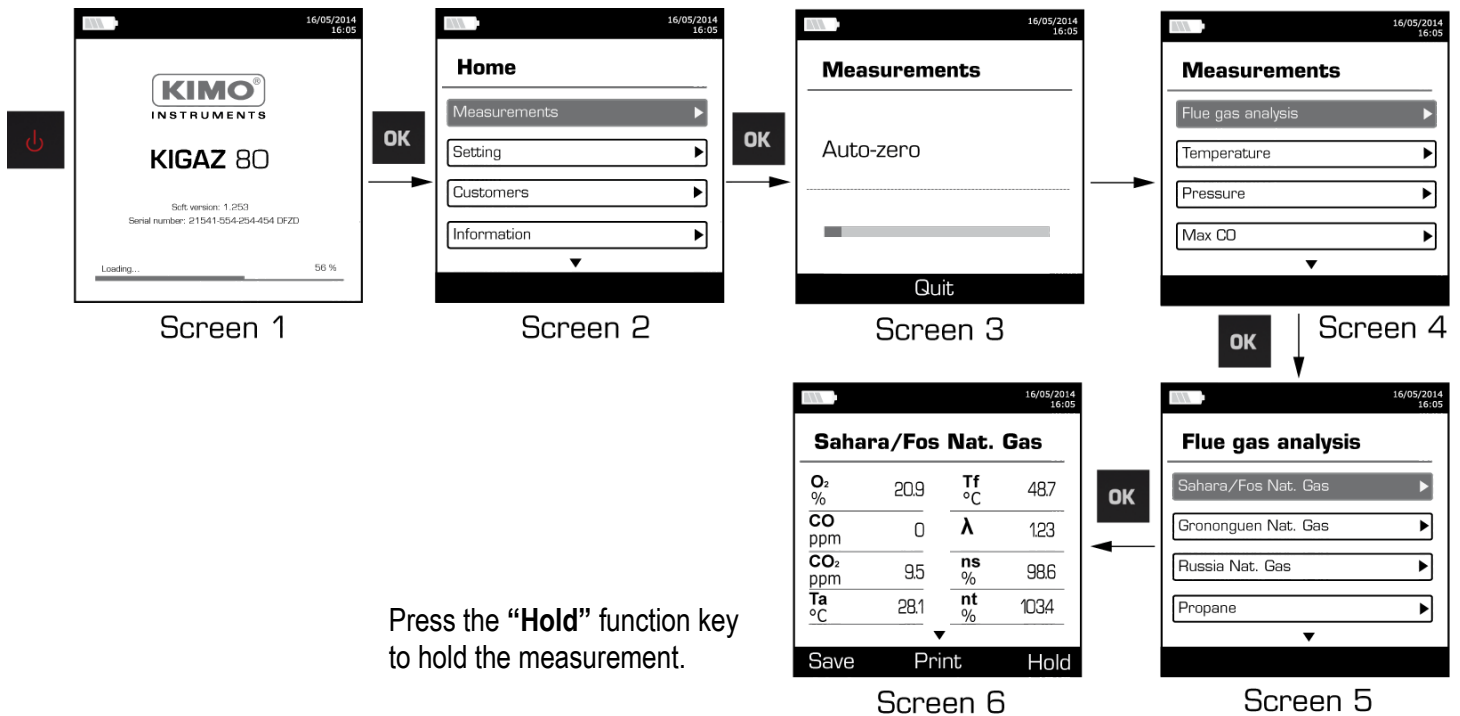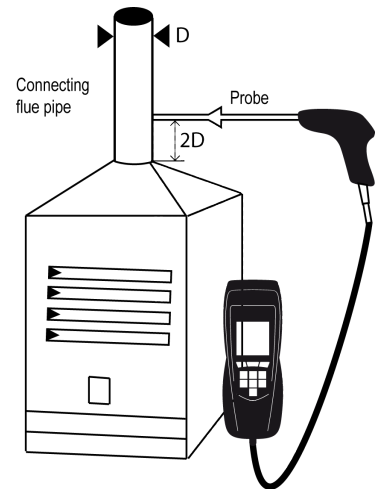


3.3. Zoom function

From the gas analysis screen, the zoom function is available using the direction arrows.

The initial screen displays 8 measured values.

- To zoom in, press the right arrow.
The screen displays 4 measured values.
- To zoom in again, press the right arrow.
The screen displays 2 measured values.
- To zoom in again, press the right arrow.
The screen displays one measured value.
- To zoom out, press the left arrow.
- At any time, press the down arrow to scroll the values.

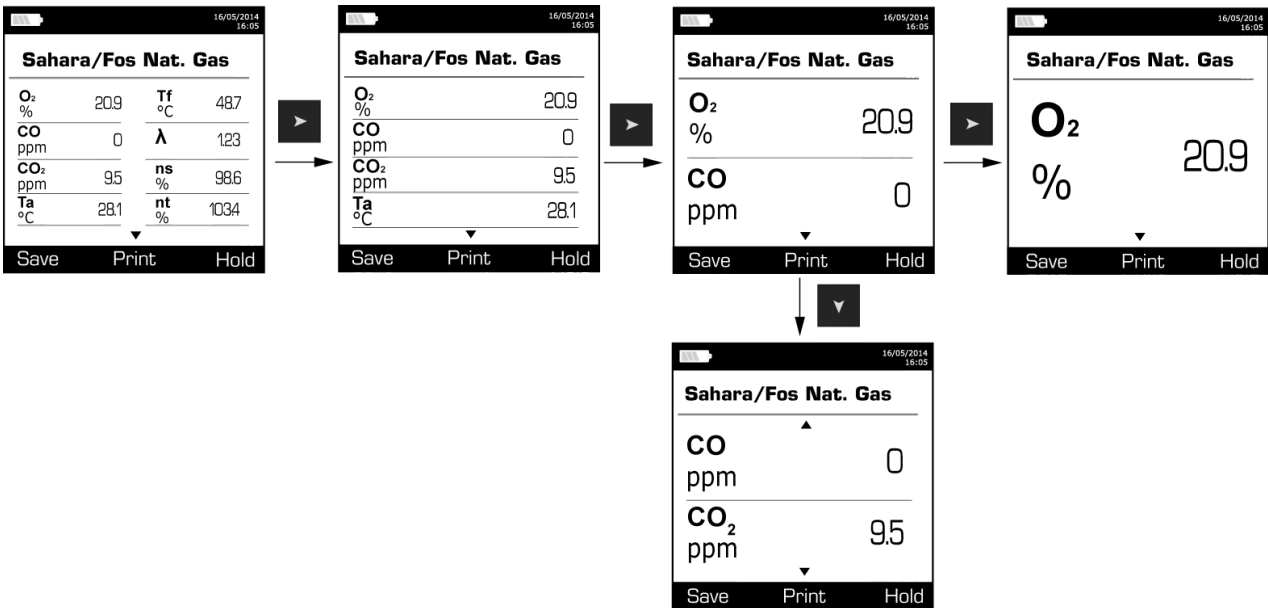

3.4. Assign the analysis to a customer

- At the end of the analysis, when measurements are constant, it is possible to assign it to a customer recorded in the analyser or to unrecorded customer that should be created.
- Press the **“Save”** function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen of the analysis.

3.5. Add the measurement to a group

The groups allow to regroup measurements in folders. The group function has to be activated (see page 18).

Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group. The group function must be activated (see page 18).

The analyser proposes to add the measurement to a group.

- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

3.6. Print the analysis results

It is possible to print the results on the ticket:

- Press the **“Print”** function button.
Results are printed on the ticket.

See page 17 for the printing configuration.

4. Set the different parameters of the analyser

The “**Setting**” menu allows to set the following parameters:

- Instrument (screen, printing, auto-off,...)
- Combustibles
- Measurements
- References (O₂, atmospheric pressure and altitude)
- Auto-zero
- Operators



The “**Setting**” part allows to set parameters that can affect the performed measurements. These settings must be made by a qualified technician.

4.1. Set the device

4.1.1. Screen settings

This part allows to set brightness and contrast of the screen from 1 to 9.

- Turn on the instrument.
Home screen is displayed.
- Go to “**Setting**” with up and down arrows then press **OK**.
- Go to “**Instrument**” then press **OK**.
The screen with the different parameters to set is displayed.
- Press **OK**.
The screen with the settings to perform appears.
- Go to the set to perform with up and down arrows then press **OK**.
- Press the left arrow to decrease **the brightness** or **the contrast** or press the right arrow to increase it.
- Press **OK** to validate.

4.1.2. Set the auto-off

The auto-off turns off the analyser automatically after some time of non-use.

It is possible to set the auto-extinction at 15 / 30 / 45 / 60 / 90 or 105 minutes or to deactivate it.

“**Setting > Instrument**” screen is displayed.

- Go to “**Auto-extinction**” with up and down arrows then press **OK**.
- Select the required time of auto-extinction or “**Off**” to deactivate it with up and down arrows.
- Press **OK**.

4.1.3. Change the language

It is possible to select the language of the instrument: French or English in standard. A third language is downloadable through the LIGAZ-2.

“**Setting > Instrument**” screen is displayed.

- Go to “**Language**” with up and down arrows then press **OK**.
- Select the language with the up and down arrows.
- Press **OK**.

4.1.4. Modify date and time

“**Setting > Instrument**” screen is displayed.

- Go to “**Date/time**” with up and down arrows then press **OK**.
- Go to the parameter to modify with left and right arrows (day, month, year, hour, minute or second).
- Press **OK**.
- Press up and down arrows to modify the selected parameter.
- Press **OK**.
- Repeat the procedure on another parameter if required.
- Go to “**Date format**” with up and down arrows then press **OK**.
- Select “**Day/Month**” to display the day then the month or “**Month/Day**” to display the month then the day then press **OK**.

- Go to “**Time Format**” with up and down arrows then press **OK**.
- Select the time format : “**12**” or “**24**”.
If 12 is selected, “AM” for ante meridiem or « PM » for post meridiem will be displayed in front of the time.
- Press the “**OK**” function key to quit the screen and save the modifications or press **Esc** to cancel.

4.1.5. Set the printing of tickets

“**Setting > Instrument**” screen is displayed.

- Go to “**Printing**” with up and down arrows then press **OK**.
- Go to “**Format**” with up and down arrows then press **OK**.
- Select the ticket format: long or short with the up and down arrows then press **OK**.

Long ticket format: prints the headers, the user name, the customer and the selected boiler, the type of device and its serial number, the type of combustible, the inspection date and time and the measurements results.

Short ticket format: prints only the device reference, the type of combustible, the date and time and the measurement results.

KIMO[®]
INSTRUMENTS

Entête 1
Entête 2
Entête 3
Entête 4
Operator : Operateur 1
Signature :

HIGAZ 80
Serial num. :
3C 150699999

Combust. :
Sahara/Fos Nat. gas
Date : 08/12/2015
Time : 15: 21: 07

Measured values	
O2	3.0 %
CO	0 ppm
Amb. T	25.3 °C
Gas T	50.1 °C

Calculated values	
CO2	11.9 %
Air exc.	1.00
Diff. T	24.8 °C
Low Eff.	99.0 %
High Eff.	104.1 %
Losses	1.0 %
Dew point	58.8 °C
CO (O2)	0 ppm
O2 ref.	21.0 %

HIGAZ 80
Serial num. :
3C 150699999

Combust. :
Sahara/Fos Nat. gas
Date : 08/12/2015
Time : 15: 21: 07

Measured values	
O2	3.0 %
CO	0 ppm
Amb. T	25.3 °C
Gas T	50.1 °C

Calculated values	
CO2	11.9 %
Air exc.	1.00
Diff. T	24.8 °C
Low Eff.	99.0 %
High Eff.	104.1 %
Losses	1.0 %

- Go to “**Logo**” then press **OK** to activate it: **ON** or deactivate it: **OFF**.
- Go to “**Header**” then press **OK**.
The keyboard appears at the bottom of the screen.
- Select the letters with the arrows then press **OK**.
- Press the “**OK**” function key to validate the header.
The keyboard disappears.
- Press **Esc** to back to “**Settings instrument**” screen and validate modifications.
 - To go from lower-case keyboard to upper-case keyboard then to numeric keyboard: press the “**A a 1**” function key.
 - To erase a letter: press the “**Delete**” function key.

4.1.6. Activate or deactivate the visual help

The visual help corresponds to help windows displayed met during a measurement procedure.

“**Setting > Instrument**” screen is displayed.

- Go to “**Help**” with up and down arrows.

- Press **OK** to activate it: **ON** or to deactivate it: **OFF**.

4.1.7. Activate the group function

Groups allow to gather measurements in a folder. To activate it:

“Setting > Instrument” screen is displayed.

- Go to **“Group”** with the keypad.
- Press **OK** to activate it: **ON** or to deactivate it: **OFF**.

For the groups creation and management, see page 18.


4.1.8. Activate or deactivate Bluetooth® function (optional)

Bluetooth® allows to communicate with the Kigaz mobile application.

“Setting > Instrument” screen is displayed.

- Go to **“Bluetooth”** with the keypad.
- Press **OK** to activate it: the box is ticked, press **OK** again to deactivate it: the box is unticked.

The  icon appears on the instrument screen when it is activated.

 When Bluetooth® is activated, the KIGAZ analyser appears with the name **“Kigaz”** in the available devices list of the computer, tablet or smartphone.

4.1.9. Select the alarm sound

“Setting > Instrument” screen is displayed.

- Go to **“Audio”** with the rotative button then press **OK**.
- Press again **OK**.
- Select with the rotative button the Alarm 1 sound or the alarm 2 sound then press **OK**.

4.2. Set the combustible

15 different combustibles are recorded in the analyser:

Sahara / Fos Natural gas	Cannel-coal
Groninguen – Natural gas	Low volatile coal
Russia – Natural gas	Coke gas
Propane	Biofuel 5%
LPG	Wood 20%
Butane	Hog fuel 21%
Light oil	Pellet 8%
Heavy fuel oil	

4.2.1. Modify a combustible

Each combustible has its own coefficient allowing to calculate losses and efficiencies in the most accurate way.



The modification of these coefficients will lead some modifications in combustion analysis results. Only a qualified technician is authorized to modify them.

It is still possible to reset the factory parameters pressing the “Factory parameters” function key or with the LIGAZ-2 software (see page 53).

“Setting” screen is displayed.

- Go to **“Combustibles”** with the arrows then press **OK**.
- Go to the required combustible with the up and down arrows then press **OK**.
- Go to the coefficient to modify with the up and down arrows then press **OK**.
The keyboard is displayed.
- Select the numbers with the arrows and press **OK** to validate.
The analyser backs to the combustibles list.
- To go from lower-case keyboard to upper-case keyboard then to numeric keyboard: press the **“A a 1”** function key.
- To erase a letter: press the **“Delete”** function key.

It is also possible to modify the name of a combustible and its type of energy (solid, liquid or gas):

“Setting > Combustibles” screen is displayed.

- Go to the combustible to modify with the up and down arrows then press **OK**.
- Press the **“Modify”** function button.
- Press **OK** on the **“Name”** line.
The keyboard appears.
- Select the letters with the direction arrows and press **OK** to validate.
- Press the **“OK”** function key to validate the new combustible name.
- Press **OK** on the **“Energy”** line.
- Select the combustible energy type: solid, liquid or gas and press **OK**.
- Press the **“Save”** function key.
The instrument backs to the combustible list with the modifications applied.

4.2.2. Add a combustible

Up to 5 combustibles can be added in the instrument's memory:

“Setting > Combustibles” screen is displayed.

- Press the **“Add”** function key.
“Add combustible” screen is displayed.
- Press **OK**.
The keyboard appears.
- Enter the name of the combustible with the keypad and press **OK**.
- Press the **“OK”** function key to validate the name of the new combustible.
- Go to **“Energy”** line with the keypad and press **OK**.
- Select **“Solid”**, **“Liquid”** or **“Gas”** with the keypad and press **OK**.
- Press the **“Save”** function key to save the new combustible.
Screen backs to the list of combustible. The new combustible is well on the list in last position. Every coefficient of the new combustible is set at 0.
- Follow the procedure of modification of combustible coefficients described page 18.

4.2.3. Delete a combustible

“Setting > Combustibles” screen is displayed.

- Go to the combustible to delete with the keypad.
- Press the **“Delete”** function key.
- Go to **YES** to confirm the deletion or go to **NO** to cancel.

4.3. Set the alarms, measurement units and CO protection

It is possible to activate an alarm for each measurement parameter. This alarm can be **rising** (the alarm of the instrument is activated when the measured value exceeds the defined threshold) or **falling** (the alarm of the instrument is activated when the measured value is below the defined threshold).

It is possible to set an alarm for the following parameters:

O₂, CO, Amb. CO, CH₄, CO₂, Q_s (losses), λ (excess air), η_t (lower efficiency), η_s (higher efficiency), T_f (flue gas temperature), T_a (ambient temperature), Pr. (pressure), ΔP (differential pressure).

4.3.1. Set the alarms

“Setting” menu is displayed.

- Go to **“Measurement”** with the keypad then press **OK**.
- Press **OK** on the **“Alarms”** line.
- Go to the parameter to modify with the keypad then press the **“Modify”** function key.
The edge (rising or falling) and the threshold of the selected parameter are displayed.
- Go to the **“Edge”** line with the keypad then press **OK**.
- Select the type of alarm with the keypad:
 - Rising edge: 🔔 ⬆
 - Falling edge: 🔔 ⬇
 - Deactivated alarm: 🔔 ✖
- Press **OK**.
- Go to the **“Threshold”** line then press **OK**

The keyboard appears.

- Enter the alarm threshold value with the keypad and press **OK** to validate.
- Validate the threshold with the “**OK**” function key.
- Validate the modifications with the “**Save**” function key.
- Press **Esc** to quit the screen.

4.3.2. Set the measurement units

It is also possible to select the measurement unit for each measured parameter:

- **Temperature:** °C, °F
 - **Draft:** Pa, inWg, hPa, mbar, mmHg, mmH₂O, psi
 - **Differential pressure:** Pa, inWg, hPa, mbar, mmHg, mmH₂O, psi
 - **CO and CO₂:** ppm, mg/m³, mg/kWh, g/kWh, g/GJ, g/m³, %
“Setting” menu is displayed.
- Go to “**Measurement**” with the keypad then press **OK**.
 - Go to “**Units**” with the keypad then press **OK**
 - Go to the parameter to modify with the keypad then press **OK**.
The list of the available units according to the parameter appears.
 - Go to the required unit with the keypad then press **OK**.
 - Press **Esc** to quit the screen.

4.3.3. Set the CO protection threshold

The CO protection allows to protect the instrument against high concentrations of CO. Above the protection threshold, the instrument will stop the pump and no other measurement will be possible. To set this threshold:

“Setting” menu is displayed.

- Go to “**Measurement**” with the keypad then press **OK**.
- Go to “**CO protection**” with the keypad then press **OK**.
- Press the “**Modify**” function key to modify the threshold.
- Enter the required threshold then press the “**OK**” function key to validate the threshold.
- Press **Esc** to quit the screen.

4.3.4. Set the display

“Setting” menu is displayed.

- Got to “**Measurement**” with the keypad then press **OK**.
- Go to “**Display**” with the keypad then press **OK**.
- Press the “**Viewable**” function key to activate or deactivate the measurement display.
- Press the “**OK**” function key to validate.

4.4. Set the references

The “**Setting > References**” screen allows to set the features of the measurement environment: O₂ reference, altitude and atmospheric pressure.

“Setting” screen is displayed.

- Go to “**References**” with the keypad then press **OK**.
- Select the parameter to modify with the keypad then press **OK**.
The keyboard appears.
- Enter the parameter value with the keypad then press **OK** to validate.

4.5. Set the duration of auto-zero and purge time

The auto-zero allows the analyser to exhaust ambient fresh air and as a result to put the sensors at 0 ppm.

“Setting” screen is displayed.

- Go to “**AutoZ/Purge**” line with the keypad then press **OK**.
The list of available duration appears.
- Go to the required duration then press **OK**.
- Press **Esc** to quit the screen.

4.6. Set the operators

It is possible to enter in the analyser names of operators who will use the instrument. The operator who performs an analysis appears on the ticket (only with the long size format).

4.6.1. Add an operator

“Setting” screen is displayed.

- Go to **“Operator”** with the keypad then press **OK**.
- Press the **“Add”** function key.
The keyboard appears.
- Enter the name with the keyboard using arrows: press **OK** to validate letters.
- Press the **“OK”** function key to validate the operator name and to add it in the list.
The analyser backs to the list of present operators.
- Press **Esc** to quit the screen.

4.6.2. Modify the operator name

“Setting” screen is displayed.

- Go to **“Operator”** with the keypad then press **OK**.
- Press the **“Modify”** function key.
The keyboard appears.
- Modify the name with the keypad: press **OK** to validate.
- Press the **“OK”** function key to validate the operator name.
The analyser backs to the list of current operators.
- Press **Esc** to quit the screen.

4.6.3. Delete an operator

“Setting” screen is displayed.

- Go to **“Operator”** with the keypad then press **OK**.
- Go to the operator to delete with the keypad.
- Press the **“Delete”** function key.
- Press **Esc** to quit the screen.

4.7. Back to factory setting of the analyser

It is possible to set the analyser with its factory setting.

“Setting > Instrument” screen is displayed.

- Press the **“Factory setting”** function key.
A message is displayed and asks to confirm the return to factory settings.
- To confirm, go to **“OK”** with the keypad then press **OK**.
- To cancel, press **Esc** or go to **“Cancel”** with the keypad then press **OK**.

4.7.1. Units and values of measurement settings of the factory setting

- **Temperature:** °C
- **Draft:** Pa
- **Differential pressure:** mbar
- **CO:** ppm
- **CO₂:** %

Alarm thresholds:


- **O₂:** 3.0 %
- **CO:** 100 ppm
- **Amb CO:** 10 ppm
- **Excess air (λ):** 1.10
- **Flue gas temperature (Tf):** 250.0 °C

Reference:

- **O₂:** 21.0 %
- **Altitude:** 800 m
- **Atmospheric pressure:** 1013.25 hPa

CO protection threshold: 2000 ppm

Duration of auto-zero and purge: 1 minute

 **Created operators and combustibles will be deleted. Created customers, boilers and inspections on boilers are not deleted after a return to factory setting.**

4.7.2. Device factory setting

Contrast: 5

Back-light: 7

Auto-off: 15 minutes

Language: French

Print: long ticket, logo display deactivated and empty headers

Visual help: ON (activated)

Alarm audio parameter: Alarm 1

Groups: OFF (deactivated)

Bluetooth (option): deactivated

5. Manage customers

It is possible to save names and addresses of different customers in the analyser. The performed measurements could be assigned to them. It is possible to create up to 100 customers.

5.1. Manage a customer

- Turn on the analyser.
- Go to “**Customers**” with the keypad then **OK**.
- Press the “**Add**” function key.
“Add customer” screen is displayed.
- Press **OK** on “**Name**” line.
The keyboard appears.
- Enter the customer name with the keypad and press **OK** to validate the letters.
- Press the “**OK**” function key.
The analyser backs to “Add customer” screen.
- Go to the 1st line of the address with the keypad then press **OK**.
- Enter the 1st line of the customer's address with the keypad and press **OK** to validate letters.
- Press the “**OK**” function key.
The analyser backs to “Add customer” screen.
- Go to the 2nd line of the address with the keypad then press **OK**.
- Enter the 2nd line of the customer's address with the keypad and press **OK** to validate letters.
- Press the “**OK**” function key.
The analyser backs to “Add customer” screen.
- Continue for both following lines of the address if necessary.
- Go to “**Phone**” line with the keypad then press **OK**.
- Enter customer's telephone number with the keypad and press **OK** to validate numbers.
- Press the “**Save**” function key.
The analyser backs to “Customer List” screen with the created new customer.

When a customer has been created, it is possible to link to this customer one or several boilers. See page 24 to create, modify and delete a boiler.

5.2. Modify a customer

- “Customers” screen is displayed.*
- Go to the customer to modify with the keypad then press **OK**.
- Press the “**Detail**” function key.
Details of the customer are displayed.
- Press the “**Modify**” function key.
- Go to the line to modify with the keypad then press **OK**.
The keyboard appears.
- Make the changes.
- Press the “**Save**” function key to validate.
The analyser backs to “Customer detail” screen.
- Press the “**Save**” function key once all the changes have been made.

5.3. Delete a customer

- “Customer” screen is displayed.*
- Go to the customer to delete with the keypad then press **OK**.
- Press the “**Delete**” function key.
A message appears asking to confirm the deletion of the customer.
- Go to **YES** then press **OK** to confirm the deletion.
- Go to **NO** then press **OK** to cancel.

6. Manage boilers

A boiler is compulsorily linked to a customer, at least one customer must be created to create a boiler. See page 23 for the creation of a customer. It is possible to link up to 10 boilers per customer.

6.1. Create a boiler

The list of customers saved in the analyser is displayed.

- Go to the customer which will be linked to the boiler with the keypad then press **OK**.
- Press the **“Add”** function key.
- Press **OK** on **“Model”** line.

The keyboard appears.

- Enter the model of the boiler with the keypad then press **OK** to validate the letters.
- Press the **“OK”** function key to validate the model.

*The analyser backs to **“Add boilers”** screen.*

- Do the same for **“Brand”**, **“Serial number”**, **“First oper. Date”**, **“Address”**, **“Location”** and **“Jet”**.
- Press **OK** on **“Tightness”** line, select **“B Type” (untight)** or **“C Type” (tight)** then press **OK**.
- Press **OK** on **“Combust.”** line, select the type of combustible for the boiler then press **OK**.
- Press **OK** to tick the **“Air pulsed burner”** box if the boiler has one.
- Press the **“Save”** function key to save the boiler features.

The analyser backs to the list of boilers.

6.2. Modify a boiler

The list of boilers saved in the analyser is displayed.

- Go to the boiler to modify with the keypad then press **OK**.
- Press the **“Detail”** function key.
- Press the **“Modify”** function key.
- Go to the line to modify with the keypad then press **OK**.

The keyboard appears.

- Make the modifications.
- Press the **“Save”** function key to validate.
- Press the **“Save”** function key once all the changes have been made.

*The analyser backs to **“Modify boiler”** screen.*

6.3. Delete a boiler

The list of boilers saved in the analyser is displayed.

- Go to the boiler to delete with the keypad then press **OK**.
- Press the **“Delete”** function key.
- *A message appears asking to confirm the deletion of the boiler.*
- Go to **YES** then press **OK** to confirm the deletion.
- Go to **NO** then press **OK** to cancel.

7. Manage the inspections

Each saved inspection is linked to a customer. It is possible to see the details of an inspection, to add one or to delete one. Available inspections in the analyser are the following: combustion, ambient temperature, flue gas temperature, internal temperature, dew-point temperature, flow/return, draft pressure, differential pressure, flue gas velocity, Max CO, opacity, ambient CO₂, ionisation current, leak detection, gas network tightness and gas flow.

The maximum number of inspections is 10 per boilers.

7.1. Get to inspections

To find every inspections of a customer and details of this inspection, follow the specified procedure:

The list of customers saved in the analyser is displayed.

- Go to the required customer then press **OK**.
Every boilers linked to this customer are displayed.
- Go to the required boiler then press **OK**.
Every inspections linked to this customer and boiler are displayed.
- Go to the required inspection then press **OK**.
Details of the inspection are displayed.

7.2. Create an inspection

It is possible to create an inspection for specific customer that will be performed later.

The list of customer's inspections is displayed.

- Press the **"Add"** function key to add an inspection.
A list of inspections is displayed.
- Go to the required inspection then press **OK**.
*The inspection is added with **"Not done"** mention.*

7.3. Delete an inspection

To delete an inspection of a customer.

The list of customer's inspections is displayed.

- Press the **"Delete"** function key to delete an inspection.
- Go to **YES** then press **OK** to delete the inspection or go to **NO** then press **OK** to cancel.

7.4. Create a group

Groups allow to gather measurements in a folder. This function has to be activated (see page 18). To create a group:

- Once the measurement is finished, press the **"Save"** function key to save it.
The analyser displays the recorded customers list.
- Select a customer with the keypad and press **OK** or create customer (see page 23) and select it.
The analyser displays the available boilers list.
- Select a boiler with the keypad and press **OK** or create a boiler (see page 24) and select it.
The analyser confirms the recording is done.
- Press **OK**.
The analyser proposes to add the measurement to a group.
- Choose **YES** to create a group: press the **"Add"** function key.
- Press **OK** to name the group.
The keyboard appears.
- Use the direction arrows to select letters and press **OK** to validate them.
- Press the **"OK"** function key to validate the name.
- Press the **"Save"** function key to save the group.
- Press **OK** to save the measurement in this group.
The instrument backs to the measurement screen.

The created group appears in the inspections list:

- Go to the **"Customer"** menu with the keypad and press **OK**.
The analyser displays the list of recorded customers on the instrument.

- Go to the required customer with the arrows and press **OK**.
The analyser displays all the boilers linked to this customer.
- Go to the required boiler with the arrows and press **OK**.
The analyser displays all the inspections linked to this customer and boiler and the created groups.
- Go to the required group folder and press **OK**.
The analyser displays the inspection list recorded in this group.
- Go to the required inspection and press **OK**.
The analyser displays the inspections details.

7.5. Add an inspection to a group

The group function has to be activated (see page 18). If an inspection or a measurement is not added to a group during the recording, it is possible to add it later:

- Go to the required inspection or measurement with the arrows.
- Press **OK** to display the details.
- Press the **“Add”** function key to add it to a group.
- Select the group to add the measurement or inspection with the arrows, or create a new group (see page 25).
- Press **OK** to validate.
The measurement is saved in the group.

7.6. Delete a group

To delete a group:

- Go to the **“Customer”** menu with the keypad and press **OK**.
The analyser displays the list of recorded customers on the instrument.
- Go to the required customer with the arrows and press **OK**.
The analyser displays all the boilers linked to this customer.
- Go to the required boiler with the arrows and press **OK**.
The analyser displays all the inspections linked to this customer and boiler and the created groups.
- Go to the required group folder and press the **“Delete”** function key.
A confirmation message is displayed.
- To confirm the deletion: go to **YES** and press **OK**. To cancel: go to **NO** and press **OK**, or press **Esc** key.

8. Perform a control of gas flow

8.1. Perform a measurement of theoretical flow

- Turn on the analyser. Go to “**Procedures**” menu with the keypad then press **OK**.
The analyser asks to select a customer: go to “OK” then press OK.
The list of customers is displayed.
- Select the customer then press **OK**.
The list of boilers is displayed.
- Select the boiler then press **OK**.
“Procedures” screen is displayed.
- Go to “**Gas flow**” with keypad then press **OK**.
A message indicating “Step 1: Theoretical flow” is displayed.
- Go to “**Next**” then press **OK**.
“Theoretical flow” is displayed.
- Specify the power capacity of the boiler in kW (data on the information plate of the boiler): go to each number, press **OK**, press the up and down arrows to **increment** or **decrement** the number then press **OK** to validate.
- Make the same operation to select the standard: **NF** or **CE**.
- Make the same operation to select the gas type: **GAS H**, **GAS B**, **BUTANE** or **PROPANE**.
- Press the “**OK**” function key to validate.
A message indicating “Step 2: Real flow” is displayed.

The theoretical flow is calculated according to a power capacity in kW of the boiler, the standard of the boiler (CE or NF standard), the gas type (Gas H, Gas B, butane or propane) and according to a coefficient. Table below allows to calculate this flow according to the power capacity:

Standard	GAS H (19-21 mbar)	GAS B (25 mbar)	Butane	Propane
NF	Pu/KW x 2.166	Pu/KW x 2.519	Pu/KW x 0.651	Pu/KW x 0.843
CE	Pu/KW x 1.927	Pu/KW x 2.241	Pu/KW x 0.579	Pu/KW x 0.750

8.2. Perform a measurement of real flow

The measurement of the theoretical flow must be performed previously
A message indicating “Step 2: Real flow” is displayed.


- Go to “**Next**” then press **OK**.
“Start index (L)” is displayed.
- Specify the start flow indicated on the gas meter: go to each number, press **OK**, press the up and down arrows to **increment** or **decrement** the number then press **OK** to validate.
- Press the “**OK**” function key to validate.
A message indicating “Step 2: Wait: 2 min.” and a progress bar are displayed.
- Wait for 2 minutes. It is possible to cancel this measurement: press **OK**.
- Go to “**Next**” then press **OK** at the end of the 2 minutes.
“End index (L)” screen is displayed.
- Specify the end flow indicated on the gas meter: go to each number, press **OK**, press the up and down arrows to **increment** or **decrement** the number then press **OK** to validate.
- Press the “**OK**” function key to validate.
A message displays the flow measurement result.

When the measurement is finished:

- Press **OK**.
The analyser asks to save the measurement result then to print the measurement result.
- Go to **YES** or **NO** then press **OK**.

8.3. Results interpretation

Read a gas meter :

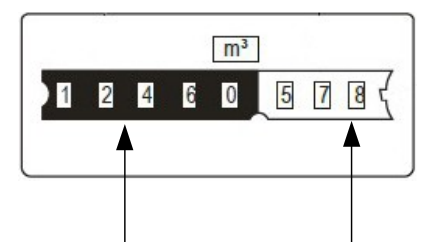

Totaliser in m³

Totaliser in litres

The analyser displays the flow result by the following:

- **OK:** lower or equal to 10%
- **A1:** between 10.1 and 20%
- **A2:** greater than 20%

9. Perform a gas network leak test

To perform this test, it is necessary to have a gas network leak testing kit. This kit is available as option (ref: KEG).

9.1. Perform the test

- Connect the different items of the kit on the network to test (see user manual of the KEG).
- Turn on the analyser.
- Go to **“Procedures”** menu with the up and down arrows then press **OK**.
The analyser asks to select a customer and a boiler: go to “OK” then press OK.
The list of customers is displayed.
- Select the customer then press **OK**.
The list of boilers is displayed.
- Select the boiler then press **OK**.
“Procedures” screen is displayed.
- Go to **“Network tightness”** with the keypad then press **OK**.
A message indicating “Plug silicone tube on P+” is displayed.
- Plug the silicone tube on P+ pressure tap then press **OK**.
A message indicating “Pressurise to 50 mbar” is displayed.
- Pressurise the network to 50 mbar then press **OK**.
A message indicating “Please wait 10 minutes” and a progress bar are displayed.
At the end of the 10 minutes, results are displayed:
 - start pressure
 - end pressure
 - possible loss of pressure

9.2. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the **“Save”** function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

9.3. Print the results

It is possible to print the results on the ticket:

- Press the **“Print”** function button.
Results are printed on the ticket.


See page 17 for the printing configuration.

10. Perform a pressure measurement


The draft measurement allows to check if the flue of the boiler correctly clears flue gas caused by the combustion.

10.1. Perform the draft measurement


- Connect the flue gas probe on the analyser.
- Turn on the analyser.
- Go to the **“Measurement”** menu with the keypad then press **OK**.
The analyser performs the gas autozero: remaining time and a progress bar are displayed on the screen.
- Go to **“Pressure”** with the keypad then press **OK**.
- Go to **“Draught pressure”** with the keypad then press **OK**.
Measurement launches and the analyser displays the draft.

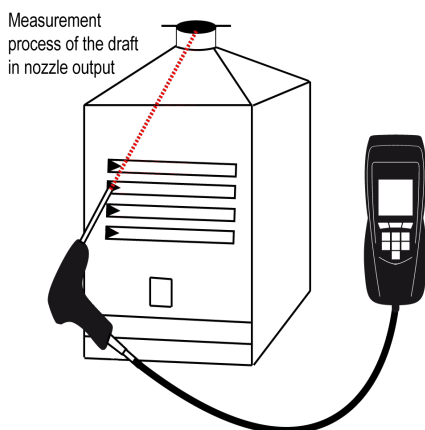

Put the probe of the KIGAZ 80 in the draft hood, going through the front face of the boiler

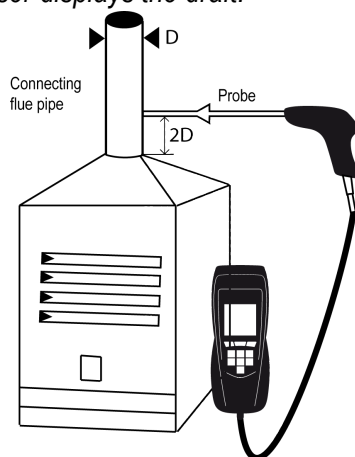

Put the probe of the KIGAZ 80 in the nozzle output, from the beginning of the connecting flue

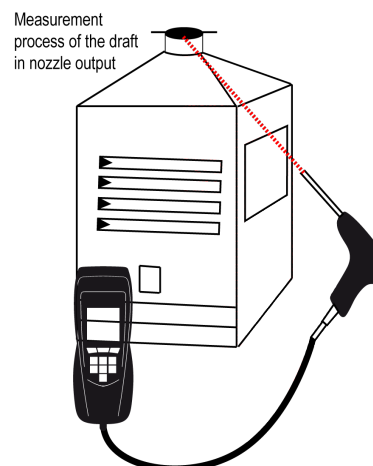

Put the probe of the KIGAZ 80 in the draft hood, going through the side openings of the boiler

10.2. Perform a differential pressure measurement

- Connect the flue gas probe on the analyser.
- Turn on the analyser
- Go to the **“Measurement”** menu with the keypad then press **OK**.
The analyser performs the gas auto-zero: remaining time and a progress bar are displayed on the screen. The pressure measurement remains possible.
- Go to **“Pressure”** with the keypad then press **OK**.
- Go to **“Diff. Press.”** with the keypad then press **OK**.
- Press **“Auto-zero”**.
Measurement launches and the analyser displays the differential pressure.

10.3. Perform a flue gas velocity measurement

- Connect a Pitot tube on the analyser (for more details, see page 36).
- Turn on the analyser.
- Go to the **“Measurement”** menu with the keypad then press **OK**.
The analyser performs the auto-zero: remaining time and a progress bar are displayed on the screen.
- Go to **“Pressure”** with the keypad then press **OK**.
- Go to **“Flue gas velocity”** with the keypad then press **OK**.
The measurement launches and the analyser displays the differential pressure.

10.4. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the **“Save”** function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.

The analyser displays the list of available boilers.

- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

10.5. Add the measurement to a group

The group function has to be activated (see page 18). Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

The analyser proposes to add the measurement to a group.

- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

10.6. Print the results

It is possible to print the results on the ticket:

- Press the **“Print”** function button.
Results are printed on the ticket.

See page 17 for the printing configuration.

11. Perform a measurement of ambient CO₂

11.1. Perform the measurement

- Connect a CO₂ probe (available as option) on C1 connection on the top of the analyser.
- Turn on the analyser.
- Go to the **“Measurement”** menu with the keypad then press **OK**.
The analyser performs the auto-zero: remaining time and a progress bar are displayed on the screen.
- Go to **“Ambient CO₂”** with the keypad then press **OK**.
Measurement launches and the analyser displays the level of ambient CO₂.

11.2. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the **“Save”** function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

11.3. Add the measurement to a group

The group function has to be activated (see page 18). Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

The analyser proposes to add the measurement to a group.

- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

11.4. Print the results

It is possible to print the results on the ticket:


- Press the **“Print”** function button.
Results are printed on the ticket.

See page 17 for the printing configuration.

12. Perform a measurement of Max CO

12.1. Perform the measurement

- Connect a CO probe (available as option) on C1 connection on the top of the analyser or connect the flue gas probe on the single connector on the bottom of the analyser.
- Turn on the analyser.
- Go to the **“Measurement”** menu with the keypad then press **OK**.
The analyser performs the auto-zero: remaining time and a progress bar are displayed on the screen.
- Go to **“Max CO”** with the keypad then press **OK**.
- Press **OK** to launch the measurement.
The measurement is launched, the instrument displays the level of CO and the level of Max CO.
When the measurement duration is finished, the analyser displays the value of maximum CO during the measurement.

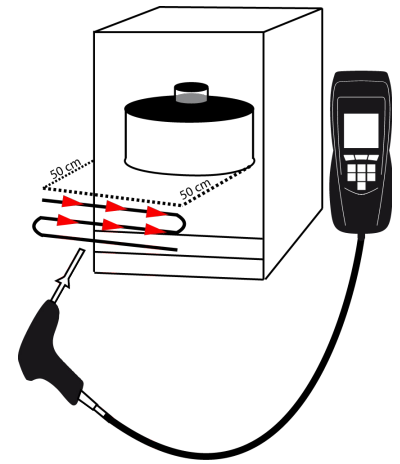

The default measurement duration is **30 s**. It is possible to change this duration before starting the measurement:

- On Max CO screen, before pressing OK to start the measurement, press the **“Duration”** function key.
“Duration” screen is displayed.
- Press **OK**.
- Use the keypad to select the required measurement duration: **30 / 40 / 50 s** or **1 / 2 / 3 / 4 / 5 minutes**.
- Press **OK** to validate the measurement duration.
- Press **Esc** to back to the screen of measurement start of Max CO.

12.2. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the **“Save”** function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

12.3. Add the measurement to a group

The group function has to be activated (see page 18).

Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

- The analyser proposes to add the measurement to a group.*
- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

12.4. Print the results

It is possible to print the results on the ticket:

- Press the **“Print”** function button.
Results are printed on the ticket.

See page 17 for the printing configuration.

13. Perform some temperature measurements

13.1. Perform a measurement of ambient temperature

- Connect a Pt100 temperature probe (available as option) on C1 connection on the top of the analyser.
- Turn on the instrument
Home screen is displayed with measurement menu highlighted.
- Press **OK**.
The analyser performs the auto-zero: remaining time and a progress bar are displayed on the screen. However it is possible to reach the temperature menu during the auto-zero.
- Go to “**Ambient Temp.**” with the keypad then press **OK**.
The temperature detected by the Pt100 probe is displayed on the analyser.

13.2. Perform a measurement of flue gas temperature

- Connect the flue gas probe on the analyser.
- Turn on the analyser.
Home screen is displayed with measurement menu at the forefront.
- Press **OK**.
The analyser performs the gas auto-zero: remaining time and a progress bar are displayed on the screen. However it is possible to reach the temperature menu during the auto-zero.
- Go to “**Flue gas Temp.**” with the keypad then press **OK**.
The screen displays the flue gas temperature detected by the thermocouple probe of the flue gas probe.

13.3. Perform an ambient temperature measurement with the internal sensor

- Turn on the instrument
Home screen is displayed with measurement menu at the forefront.
- Press **OK**.
The analyser performs the auto-zero: remaining time and a progress bar are displayed on the screen. However it is possible to reach the temperature menu during the auto-zero.
- Go to “**Internal Temp.**” with the keypad then press **OK**.
The screen displays the NTC temperature detected by the analyser.

13.4. Perform a Flow/Return temperature measurement

- Connect a thermocouple Velcro type (ref. : SKV 150) or lamella contact (ref. : SKCT) probe on the Kigaz.
- Turn on the instrument.
Home screen is displayed with measurement menu highlighted.
- Press **OK**.
The analyser performs the auto-zero: remaining time and a progress bar display on the screen. However it is possible to reach the temperature menu during the auto-zero.
- Go to “**Flow/Return Temp.**” with the keypad then press **OK**.
The screen displays the T1 temperature and the T2 temperature and the delta of temperature (ΔT) detected by the analyser.

13.5. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the “**Save**” function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

13.6. Add the measurement to a group

The group function has to be activated (see page 18). Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

The analyser proposes to add the measurement to a group.

- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

13.7. Print the results

It is possible to print the results on the ticket:

- Press the **“Print”** function button. *Results are printed on the ticket.*

See page 17 for the printing configuration.

14. Perform a measurement of opacity

It is possible to enter in the analyser from 1 to 3 opacity indexes performed thanks to opacity pump available as option. The opacity index consists of the measurement of solid waste of combustion in the flue with a pump and a filter of measurement. The filter coloration is compared with a table reference composed by 10 greyed areas numbered from 0 to 9.

14.1. Perform the measurement



Preliminary operation: To avoid the condensation in the pump, it is necessary to breathe in WITHOUT FILTER fresh air before performing a measurement.

- Put the paper filter in the pump.
- Pump out flue gas in the middle of the flue.
The necessary gas volume for a measurement of opacity corresponds to about 10 pump aspirations.
- Compare the filter clogging to the reference table to determine the opacity index.
- Make the same operation several times if necessary, replace the filter each time.

14.2. Enter the indexes in the analyser

When the measurement of opacity has been performed, enter the opacity indexes in the analyser:

- Turn on the analyser.
The analyser performs the auto-zero: remaining time and a progress bar are displayed on the screen. However it is possible to reach the Bacharach index menu during the auto-zero.
- Press **OK**.
- Go to “**Bacharach index**” with the keypad.
- Press **OK**.
- Press **OK** on “**Index 1**” line.
- Increment the index from 0 to 9 with the keypad.
- Press **OK**.
- Repeat the procedure for 2 and 3 indexes.
*The analyser indicates the opacity indexes average on “**Average**” line at the bottom of the screen.*

14.3. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the “**Save**” function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

14.4. Add the measurement to a group

The group function has to be activated (see page 18). Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

- The analyser proposes to add the measurement to a group.*
- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

14.5. Print the results

It is possible to print the results on the ticket:

- Press the “**Print**” function button.
Results are printed on the ticket. See page 17 for the printing configuration.

15. Perform a measurement of ionisation current

The measurement of ionisation current allows to check the presence of the flame. In standard operation, the ionisation probe produces a current of a few μA or a few dozen of μA . In case of lack of flame, this current is not present anymore (measurement: 0 μA), the safety equipments of the boiler cut off the power supply.

15.1. Perform the measurement

- Connect an ionisation current probe on C1 connection of the analyser.
- Turn on the analyser.
Home screen is displayed with measurement menu at the forefront.
- Press **OK**.
The analyser performs the autozero: remaining time and a progress bar are displayed on the screen. However it is possible to reach the ionisation current menu during the autozero.
- Go to “**Ionisation current**” with the keypad then press **OK**.
- Connect the ends of the probe on the boiler.
The measured ionisation current is displayed on the analyser. This value must be equal to several dozen of μA .

15.2. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the “**Save**” function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

15.3. Add the measurement to a group

The group function has to be activated (see page 18).

Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

- The analyser proposes to add the measurement to a group.*
- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

15.4. Print the results

It is possible to print the results on the ticket:


- Press the “**Print**” function button.
Results are printed on the ticket.

See page 17 for the printing configuration.

16. Perform a flue gas velocity measurement with a Pitot tube



The used Pitot tube must be a Pitot tube type L with K thermocouple connection.

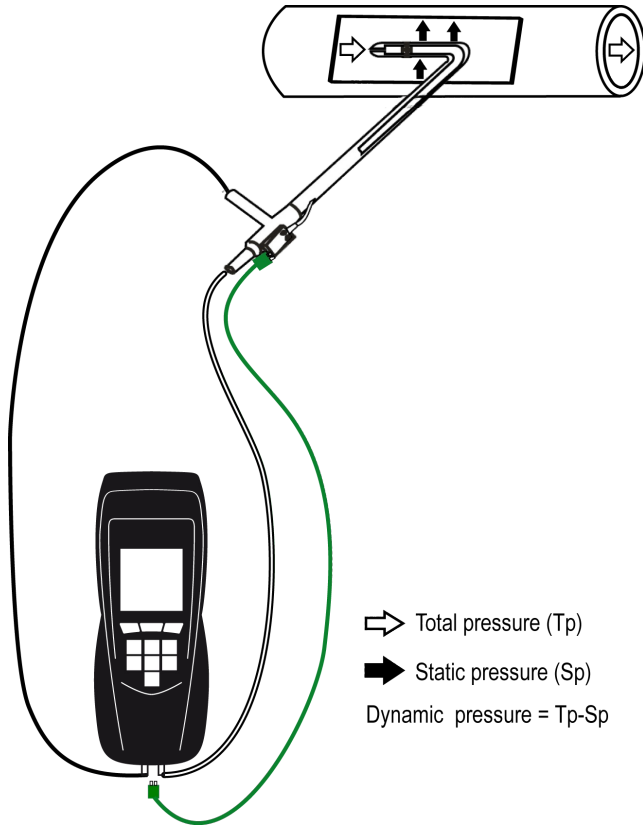

The Pitot tube must be introduced perpendicularly, in the middle into the duct and parallel to the flow. The head (ending with an ellipsoidal nose) must be maintained parallel and facing the flow. The total pressure (+) caught by the nose, is connected to the P+ at the bottom of the analyser. The static pressure (-) caught by the holes of the head, is connected to the P- at the bottom of the analyser. The connection cable of the thermocouple K probe is connected to the T1 K thermocouple inlet of the top of the analyser.



If no K thermocouple cable is connected, no value is displayed.

When the connections are made:

- Turn on the analyser.
- Go to “**Measurement**” menu then press **OK**.
- Go to “**Pressure**” menu then press **OK**.
- Go to “**Flue gas velocity**” then press **OK**.

The analyser displays the measured values.

16.1. Link the measurement to a customer

When the measurement has been performed, it is possible to link it to a customer registered in the analyser or to a customer unregistered in the analyser that must be created.

- Press the “**Save**” function button.
The analyser displays the list of recorded customers.
- Select a customer with up and down arrows then press **OK** or create a customer (see page 23) then select it.
The analyser displays the list of available boilers.
- Select the boiler with up and down arrows then press **OK** or create a boiler (see page 24) then select it.
The analyser backs to the measurement screen.

16.2. Add the measurement to a group

The group function has to be activated (see page 18). Once the measurement is linked to a customer and a boiler, it is possible to add it in a group in the instrument, or create a group:

The analyser proposes to add the measurement to a group.

- Go to **YES** and press **OK**.
- Go to the required group with the arrows and press **OK**, or create a group (see page 25).
The analyser backs to the measurement screen.

16.3. Print the results

It is possible to print the results on the ticket:

- Press the “**Print**” function button.
Results are printed on the ticket.

See page 17 for the printing configuration.

17. To get to information about the analyser

The “**Information**” menu of the analyser allows to get to several information:

- Type of analyser
- Version of the firmware
- Serial number of the analyser
- The adjustment date
- Phone and fax numbers, e-mail of Kimo Instruments
- Options of the analyser
- Type of sensor, its serial number and its installation date.


To get to this menu:

From the home screen:

- Go to “**Information**” menu with the keypad then press **OK**.
The information is displayed on the screen.
- Use the keypad to go from one screen to the other.

From any information screen:

- Press the “**Diagnostic**” function key.
The analyser displays information about sensors.

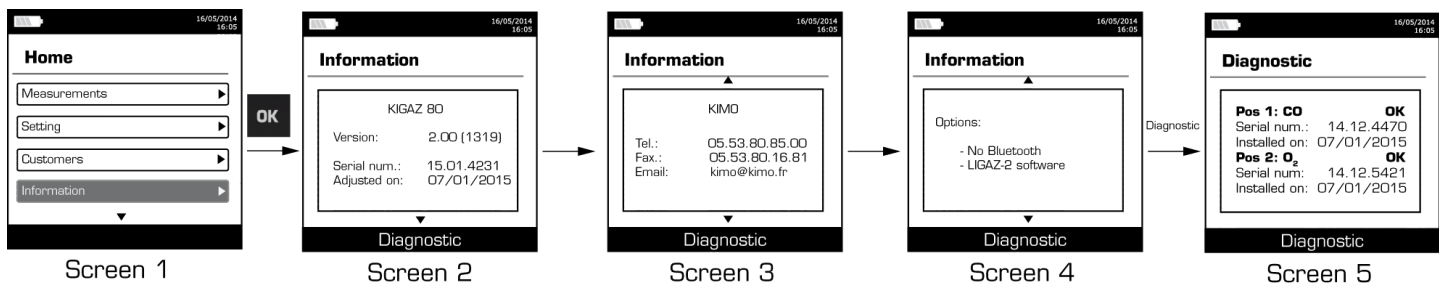

18. Maintenance of the analyser

18.1. Life-time of the sensors

Sensors are electrochemical type: inside them, in the presence of gas to detect, a chemical reaction occurs that causes an emission of electrical current. The electric current strength detected by the instrument is converted into a corresponding gas concentration. The life-time of the sensor is strongly linked to the reagent consumption present in the sensor. As their consumption increases, features of the sensor are getting worse until their exhaustion, after which it is necessary to replace it. To ensure the measurement accuracy, sensors have to be calibrated only in Assistance centre qualified by Kimo.

Sensor	Average life-time	Required calibration
O ₂	5 years	Annual
CO-H ₂	2 to 3 years	Annual

18.2. Replace the sensors

Follow this procedure to replace a used sensor:


The analyser must be turned off.


- Remove the protective cover.
- Turn the analyser.
- Unscrew the sensors cover with a flat screwdriver.
- Remove the trap.
- Disconnect the ribbon cable of the sensor to replace.
- Rotate the sensor counter clockwise taking care not to bring pressure on the board of the sensor.
- Remove the sensor.
- Put the new sensor taking care to insert the two jacket hooks of the sensor in their location.



Exercise the rotation constraint on the sensor body and not on the electronic card.

- Rotate the sensor clockwise.
- Reconnect the ribbon cable of the sensor.

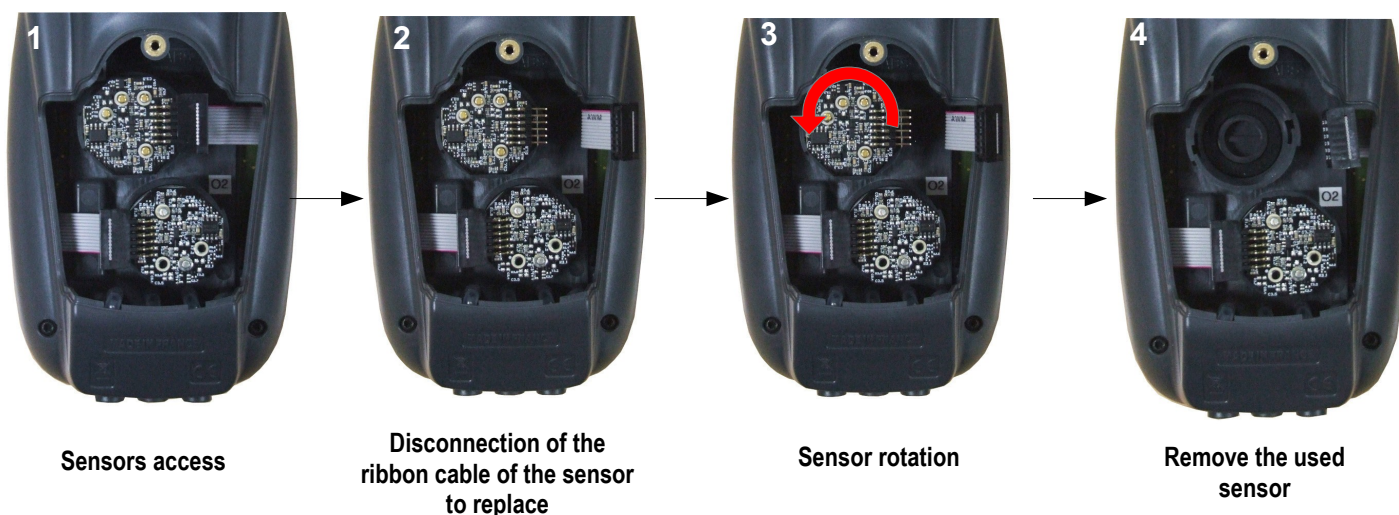

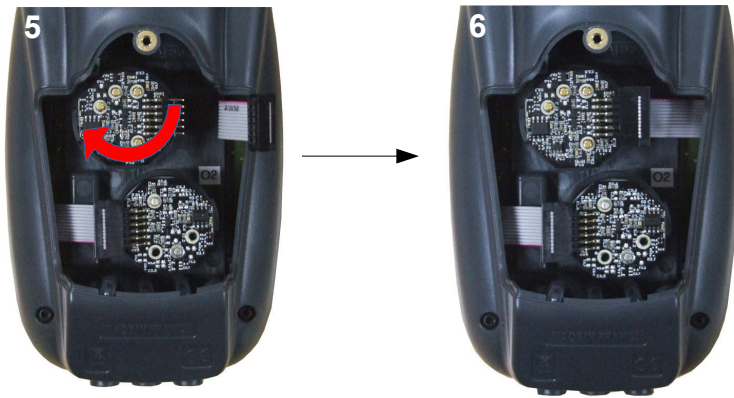

Insertion of a new sensor then rotation of the sensor

Connection of the sensor ribbon cable



Exercise the pressure on the sensor body and not on the electronic card.



Sensors have very accurate locations, see below locations defined for each sensor:

- **O₂** sensor must be in **O₂** position
- **CO-H₂** sensor must be in **CO** position



When a sensor has been replaced, it is possible to check the proper functioning of this new sensor by going in the “**Information**” menu of the analyser. It is normal that a sensor that has just been installed gives the following message: “**Current Error**”, it is necessary to wait a few time to stabilise the polarisation of the sensor. Here are the stabilization times for each sensor:

- **O₂**: 48 hours
- **CO-H₂**: 48 hours

18.3. Replace the battery

Follow this procedure to replace the battery:

The analyser must be turned off.

- Remove the protective cover.
- Turn the analyser.
- Unscrew the battery cover with a cross-head screwdriver.
- Remove the battery cover.
- Disconnect the battery.
- Connect the new battery.

19. Calculations of the different parameters

19.1. CO conversion

$$CO\left[\frac{mg}{m^3}\right] = CO[ppm] \times 1.24922$$

$$\lambda = \frac{CO_{2max}}{CO_2} = \frac{21}{21 - O_2}$$

$$CO\left[\frac{mg}{kWh}\right] = CO\left[\frac{mg}{m^3}\right] \lambda \frac{V_f}{PCI \times 0.277778}$$

$$CO\left[\frac{g}{kWh}\right] = CO\left[\frac{mg}{m^3}\right] \lambda \frac{V_f}{PCI \times 0.277778} \times 0.001$$

$$CO\left[\frac{g}{GJ}\right] = CO\left[\frac{mg}{kWh}\right] \lambda \frac{V_f}{PCI \times 0.277778} \times 0.001$$

$$CO\left[\frac{mg/m^3}{O_{2ref}}\right] = CO\left[\frac{mg}{m^3}\right] \times \frac{21 - O_{2ref}}{21 - O_2}$$

$$CO\left[\frac{ppm}{O_{2ref}}\right] = CO[ppm] \times \frac{21 - O_{2ref}}{21 - O_2}$$

$$CO[\%] = CO[ppm] \times 0.0001$$

$$CO\left[\frac{g}{m^3}\right] = CO\left[\frac{mg}{m^3}\right] \times 0.001$$

With:

- O_{2ref} a reference value selected by the user, this value has to be entered in the device in %.
- O_2 oxygen value measured in %.
- V_f the theoretical volume of flue gas in m^3 (given in the table of coefficient)
- NCV the net calorific value in MJ (given in the table of coefficient)
- CO_{2max} the maximum level in % in carbon dioxide of flue gas dry products (given in the table of coefficient)

19.2. Calculation of flue gas velocity


$$V = k \sqrt{\frac{2 \Delta P}{M_{VF}}}$$

With:

- k: coefficient of the differential pressure item
- ΔP : differential pressure (dynamic pressure).
- M_{VF} : mass density of the flue gas (already calculated for the calculation of the higher efficiency).

LIGAZ-2

Logiciel d'exploitation
Operating software

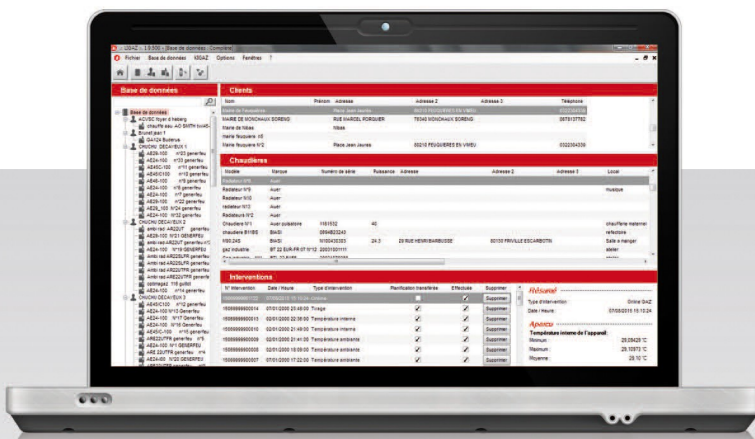

Notice d'utilisation / User manual

1. Introduction

LIGAZ-2 software, supplied with the gas analysers of the KIGAZ range, allows to set the analyser, to create and give information a customers, boilers and inspections database, to process and download measurement datasets.

2. Software installation


2.1. Recommended minimum configuration

For the proper functioning of the software, the following minimum configuration is recommended:


- **Operating system:** Windows, XP, VISTA, 7
- **Communication port:** USB 2.0
- **DVD player**
- **RAM memory:** 1 GO
- **Disk memory:** 1 GO


2.2. Installation

- Put the DVD into the player of the computer.
It automatically starts. If not, go to "My computer", double-click on DVD drive then on "SetupLIGAZ-2" icon.
- Follow the indications of installation.

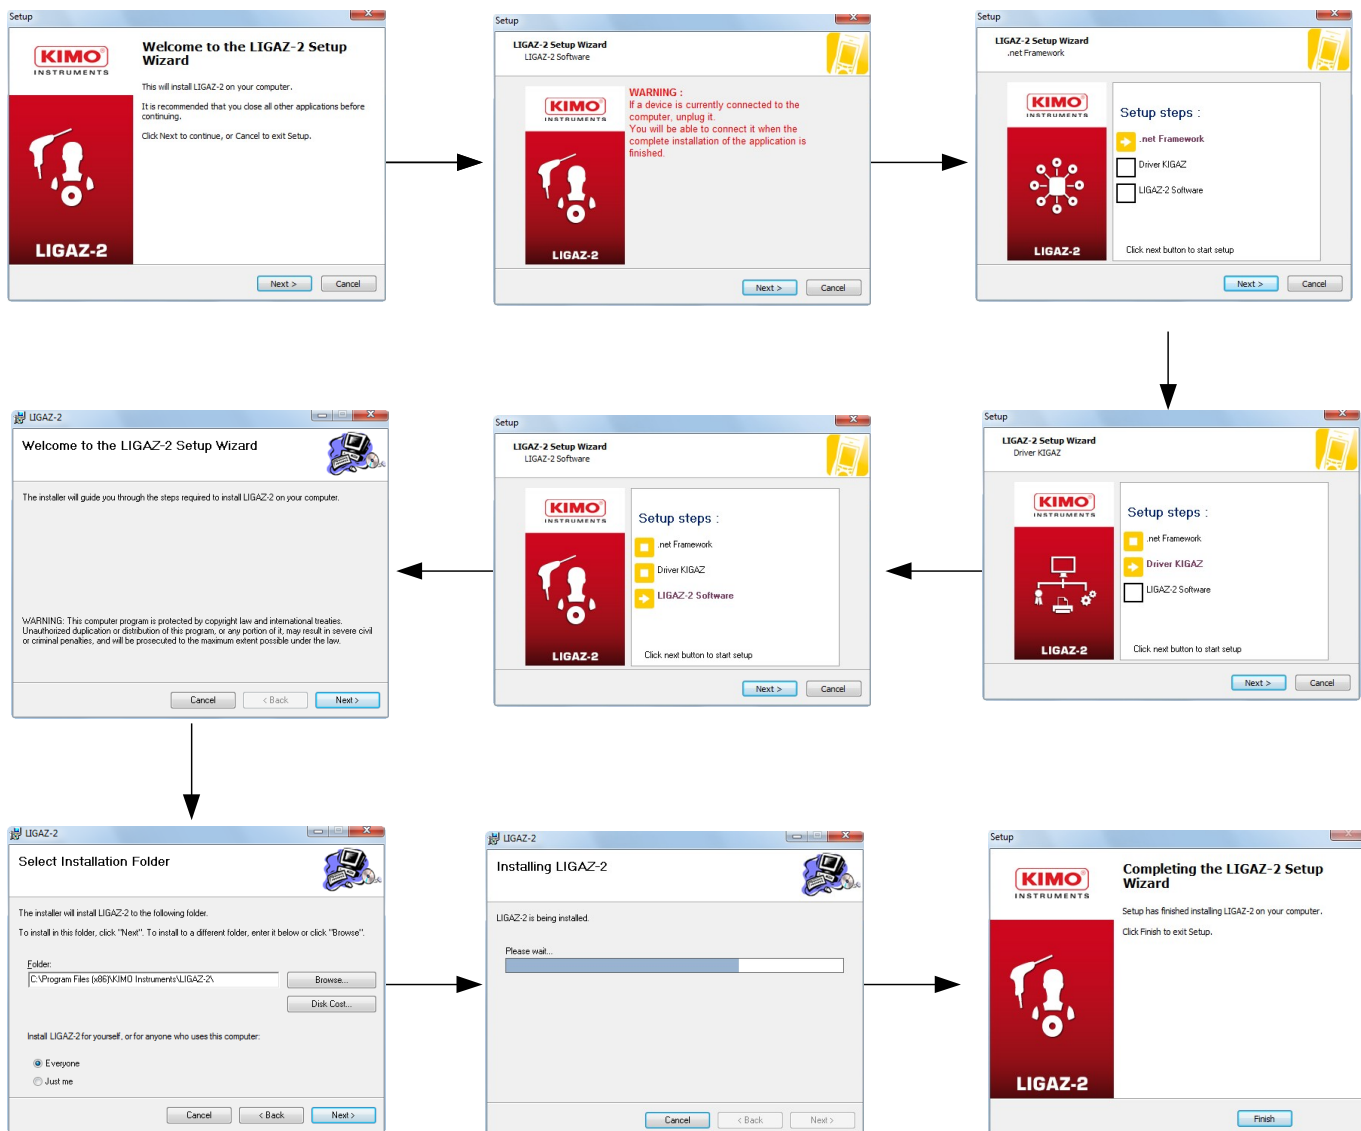

3. Start with the software

After double-clicking on the  software launching icon on the desktop, the homepage of the software opens:

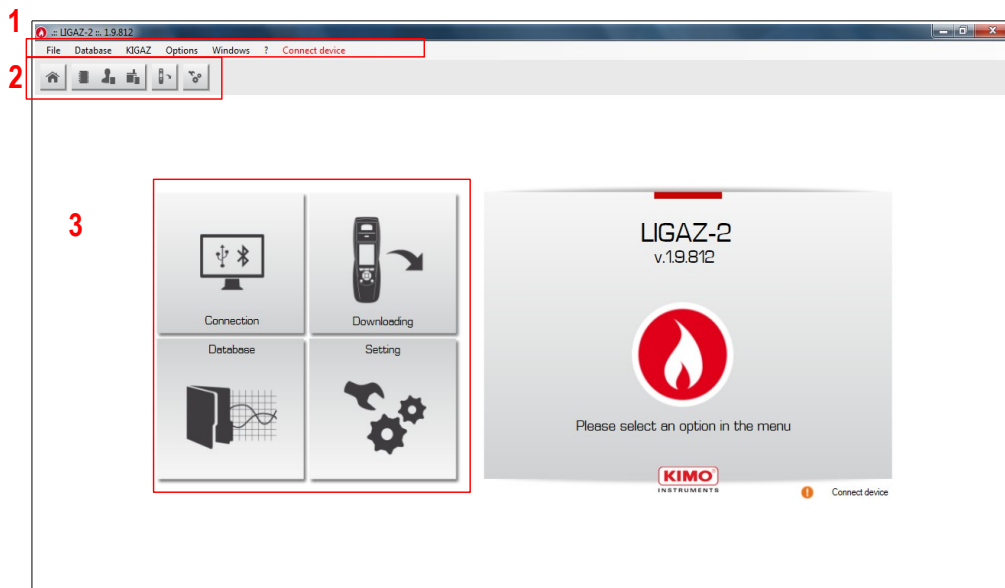

3.1. Meaning and functions of the menu bar (1)

➤ File

- **Back to homepage:** reduce all the opened windows
- **Save database:** save the database into the computer
- **Import database:** import a LIGAZ-2 or LOGAZ-2 (optional software) database saved into another computer
- **Quit:** close the software

➤ Database

- **Total:** opens the total database window (Customers, boilers and performed inspections)
- **Customers:** opens the customers database window
- **Boilers:** opens the boilers database window
- **Database setting:** opens the saving setting window of the database (location and recurrence)

➤ KIGAZ

- **Downloading:** allows to download data saved in the analyser and the instrument setting
- **Setting:** allows to set different parameters (autozero, combustibles, references...)
- **Customers / boilers deletion...:** allows to delete customers and/or boilers saved in the analyser
- **Comparison of PC elements with KIGAZ...:** allows to compare information on customers and boilers between the LIGAZ-2 database and the analyser

➤ Options

- **E-mail:** allows to set parameters to send emails
- **User:** information about the user
- **Languages:** allows to select the software language (French or English)







➤ Windows: allows to go from one window to another

➤ ?:

- **User manuals:** allows to get to software and analyser user manuals
- **Hotline:** allows to get to the address and fax and phone number of the company or send a report to the after sales service
- **About:** indicates software version and database version

➤ Device connection: indicates the connection state of the device connection. “Connect device” or “Device connected”.

3.2. Meaning and functions of tool bar buttons (2)


 Back to homepage: closes all the opened windows	 Opens the boilers database window
 Opens the complete database window (Customers, Boilers, Inspections)	 Opens the analyser download window
 Opens the customer database window	 Opens the analyser setting window


3.3. Meaning and functions of the homepage buttons (3)


 Allows to connect the analyser to the software	 Allows to connect the analyser and access the inspections unload window
 Allows to access the complete database: Customers, boilers and inspections	 Allows to access the analyser setting


4. Download inspections


Inspections stored in the analyser can be downloaded on the computer:

- Connect the analyser to the computer thanks to the supplied USB cable and **turn on the analyser**.
- Launch **LIGAZ-2** software.
- Connect the analyser to the **LIGAZ-2** software clicking on the  homepage button. *The software indicates that connexion is successful.*

- Click on the download homepage button  Or
- Click on “**KIGAZ**” menu then on “**Downloading**”.
- Or

- Click on the download icon of the tool bar  *The software recovers inspections contained in the analyser. This operation can take a few minutes. At the end of the recovery, the following window is displayed:*

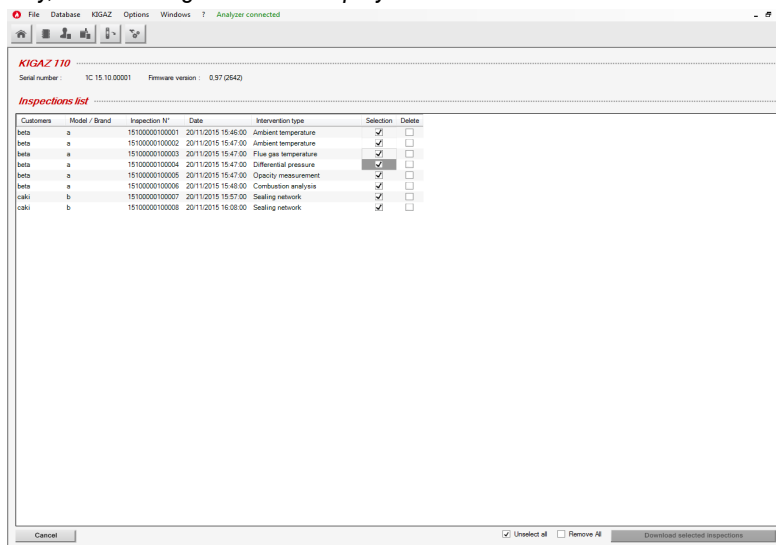


- Tick the boxes corresponding to the inspections to download on the computer. To delete an inspection from the instrument, tick the “**Delete**” box. To download an inspection to add to your database and delete it from the instrument, tick both boxes.
- Click on the  button. *A message indicates that the transfer started, then the message “**Transfer done**” is displayed: the dataset has been downloaded successfully.*
- Click on **OK**. *The “**Complete database**” window is displayed with the new inspections downloaded. Customers and boilers linked to the downloaded inspections are added to the “**Customers**” and “**Boilers**” databases.*

5. Use the different databases


Databases are used to give information about features of boilers and customers. **LIGAZ-2** software allows to recover customers and boilers created in the analyser and allows to transfer customers and boilers created with **LIGAZ-2** software in the analyser.

- Launch the software by double-clicking on the  icon in the desktop.
- These databases are saved in the hard disk of the computer. See page 48 for the “**Database settings**”.

5.1. Use the customer database


- Click on the  button of the tool bar or click on “**Database**” menu, then on “**Customer**”.

The following window is displayed:

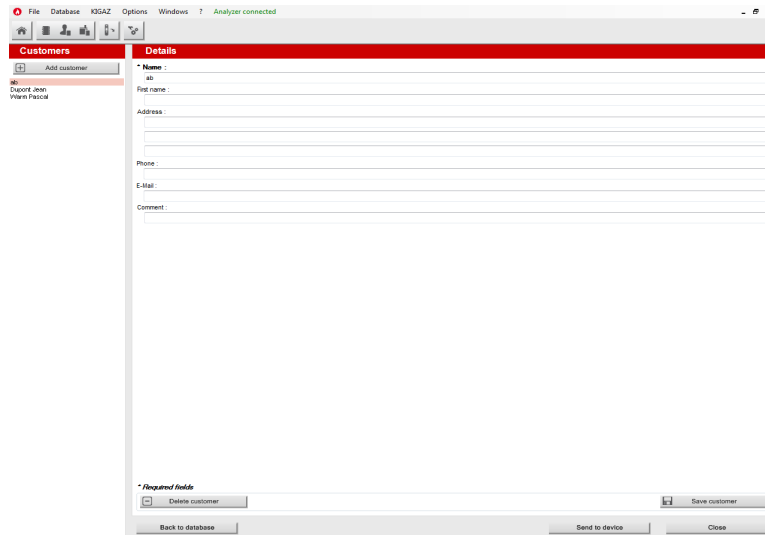


The fields are not accessible.


The customer list created on the device are displayed on the left of the screen.


- To add a customer, click on the  button.




The fields become accessible.

- Fill in the different fields. The “**Name**” field is required.
- To save it, click on the  button.
- A confirmation message is displayed.
- Click on **OK**.

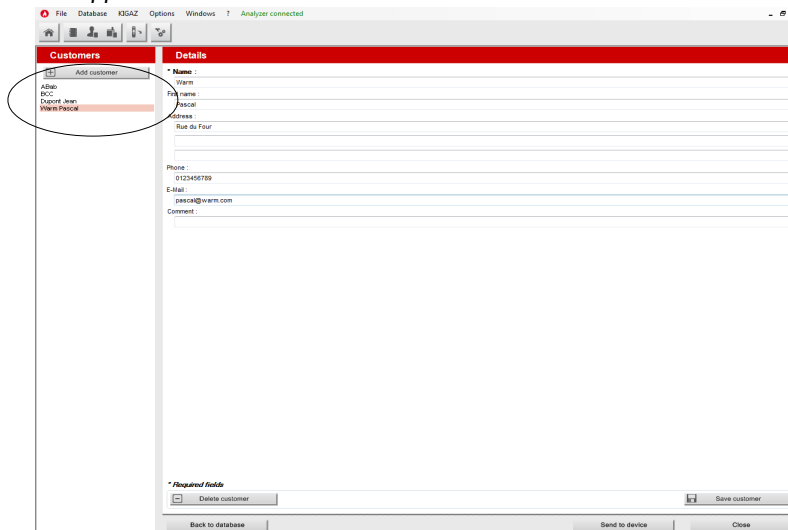The created customer appears in the list on the left of the screen:




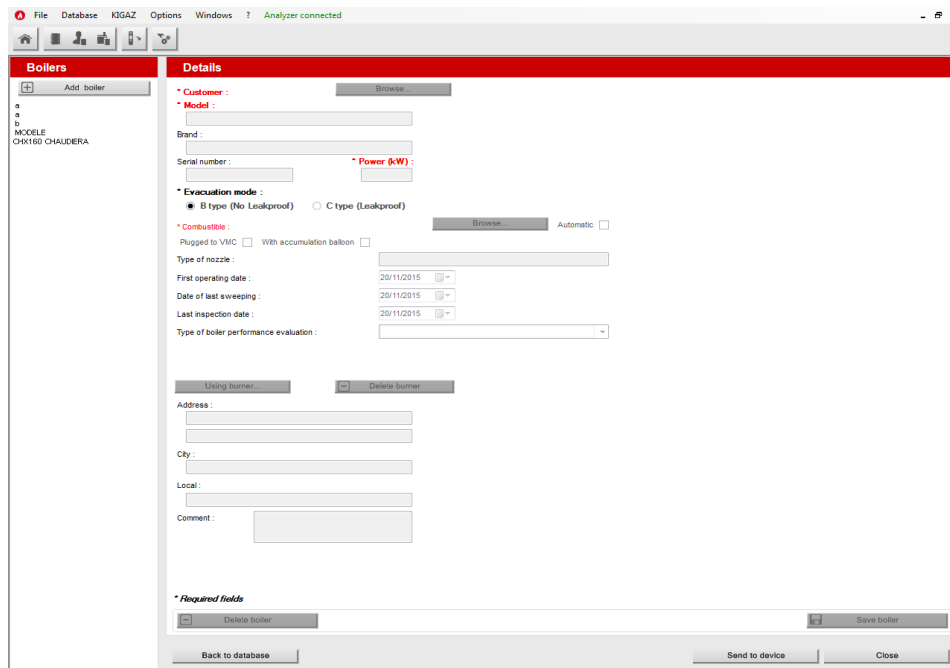
- Repeat the procedure to add other customers.
- To transfer a customer to the analyser, select it on the customer list on the left of the screen and click on the following button: . If it is inaccessible, check the device connection.
- A message confirms the successful transfer.
- Click on **OK**.

- To download customers from the analyser to the software database, it is necessary to download inspections present on the device (see page 54). Only the customers linked to an inspection are added to the **“Customers”** software database. The boilers linked to this customer are also added to the **“Boilers”** software database.
- To delete a customer, select it in the customer list and click on the  button.
A confirmation message is displayed:
- Click on **YES** to confirm the deletion, or on **NO** to cancel.
- Click on the  button to close the window and back to the homepage or on the  button to access the complete database.




5.2. Use the boilers database


Each customer can have several boilers.


- Click on the  tool bar button, or on **“Database”** menu then choose **“Boilers”**.
The following window opens:




*All the fields (type, model, power...) are inaccessible and the **“Browse”** button is inactive.*





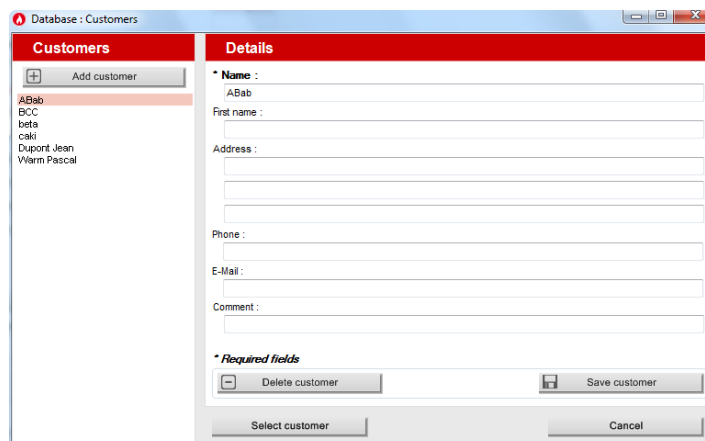
- To add a boiler, click on the  button.
The fields become accessible and the  button is active.
- Fill in the different required fields (customer, model, power in kW and combustible) as indicated below.
- Click on the  button in front of the **“Customer”** field to link the boiler to a customer.
The following window is displayed:




- Select the required customer in the list on the left then click on the  button.
The software back to the previous screen.
- Fill in the **“Model”** and **“Power”** required fields.

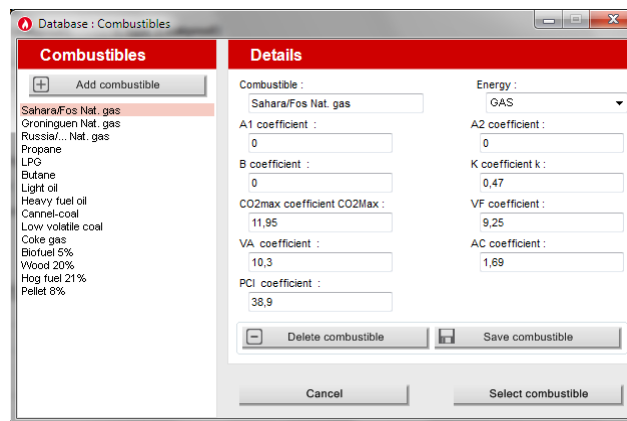



- Click on the  button in front of “**Combustible**” and select the combustible type of the boiler.
The following window is displayed:



- Select the combustible used by the boiler and click on the  button.
15 types of combustible are programmed. If the combustible type used by the boiler is not available in the list, click on the  button, fill in the fields, click on the  button then on the  button.
- To save the boiler, click on the  button.
The software displays a confirmation message.
- Click on **OK**.

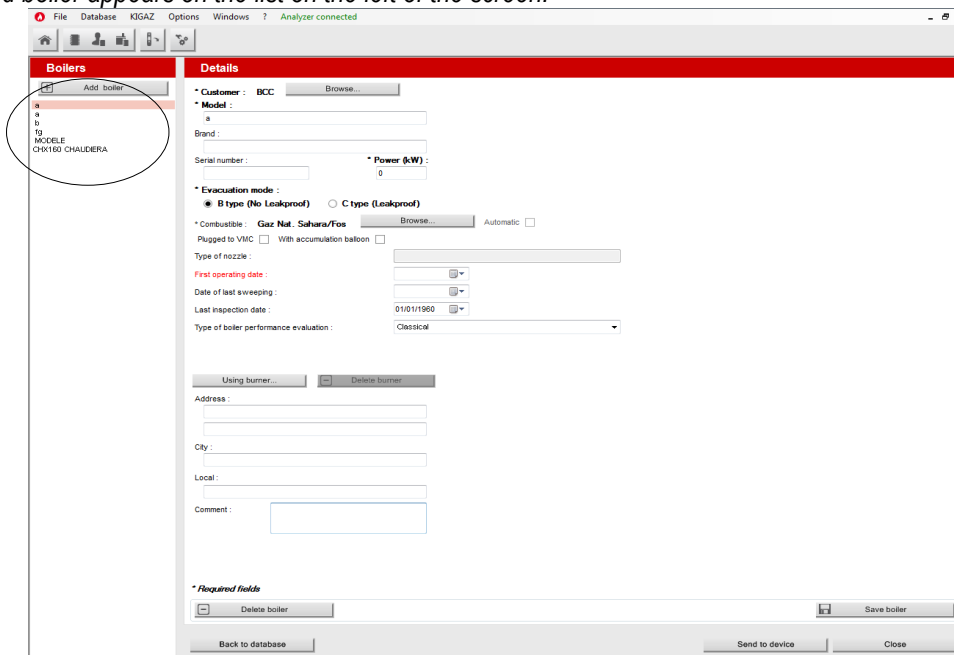

The created boiler appears on the list on the left of the screen:




- Repeat the procedure to add other boilers.
- To transfer a boiler to the analyser, select it on the boilers list then click on the  button. If it is not accessible, check the device connection.
A message is displayed to confirm the transfer:
- Click on **OK**.
- To download boilers from the analyser to the software database, it is necessary to download inspections present on the device (see page 54). Only the boilers linked to at least an inspection are added to the “**Boilers**” software database. The customer linked to this boiler is also added to the “**Customers**” software database.
- To delete a boiler, select it on the boilers list then click on the  button.
A confirmation message is displayed.
- Click on **YES** to confirm deletion or **NO** to cancel.
- Click on the  button to close the window and back to the homepage, or on the  button to access to the complete database.

5.3. Complete database

This database allows to have a global view of all customers and their boilers with also the inspections.

- Click on the  tool bar button or directly on the  button on the homepage.
 - Or
 - Click on “Database” menu, then choose “Complete”.
- The following window is displayed:

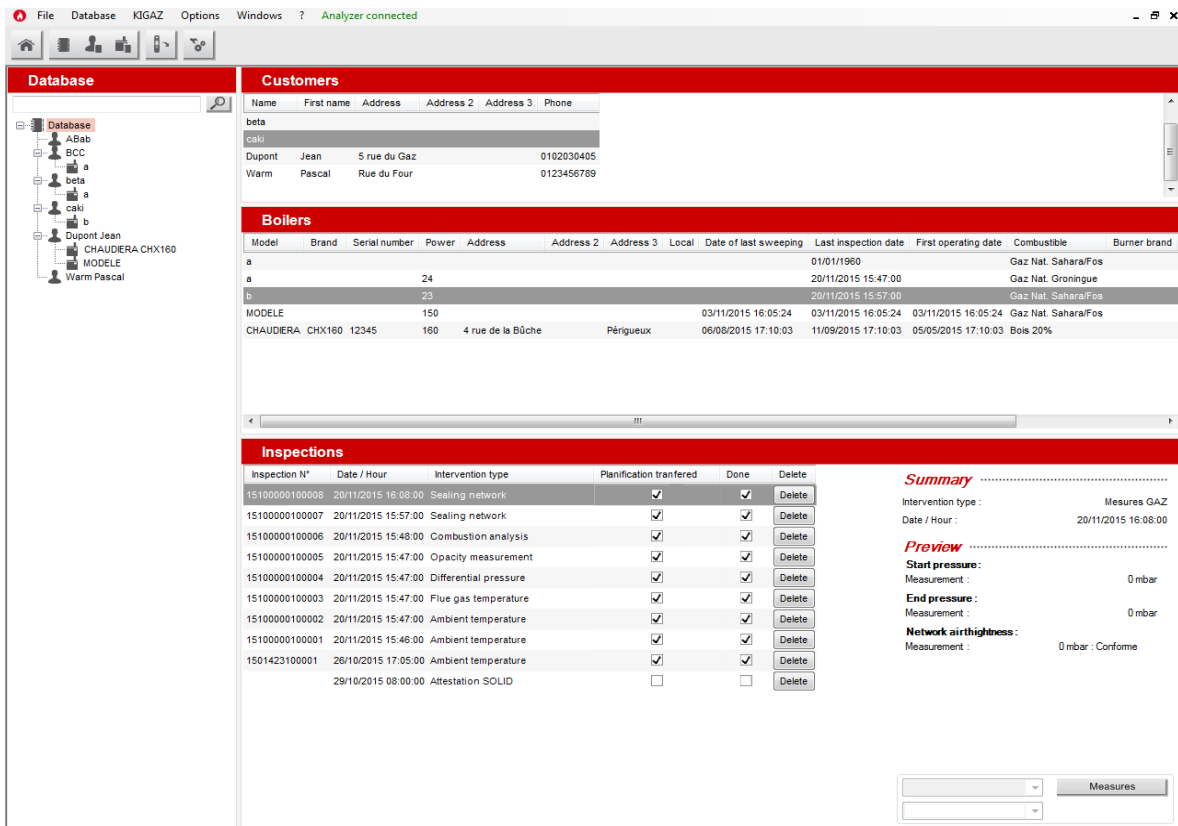

The screenshot shows the LIGAZ-2 software interface with the following sections:

- Database:** A tree view on the left showing the database structure with folders for 'Database', 'ABab', 'ccc', 'beta', 'caki', 'Dupont Jean', 'CHAUDIERA CHX160', 'MODELE', and 'Warm Pascal'.
- Customers:** A table listing customer information.


Name	First name	Address	Address 2	Address 3	Phone
beta					
caki					
Dupont	Jean	5 rue du Gaz			0102030405
Warm	Pascal	Rue du Four			0123456789
- Boilers:** A table listing boiler information.

Model	Brand	Serial number	Power	Address	Address 2	Address 3	Local	Date of last sweeping	Last inspection date	First operating date	Combustible	Burner brand
a			24					01/01/1960			Gaz Nat. Sahara/Fes	
b			23					20/11/2015 15:47:00			Gaz Nat. Groningue	
MODELE		150						03/11/2015 16:05:24	03/11/2015 16:05:24	03/11/2015 16:05:24	Gaz Nat. Sahara/Fes	
CHAUDIERA	CHX160	12345	160	4 rue de la Bûche	Périgueux			06/08/2015 17:10:03	11/09/2015 17:10:03	05/05/2015 17:10:03	Bois 20%	
- Inspections:** A table listing inspection records.


Inspection N°	Date / Hour	Intervention type	Planification transférée	Done	Delete
15100000100008	20/11/2015 16:08:00	Sealing network	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100007	20/11/2015 15:57:00	Sealing network	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100006	20/11/2015 15:48:00	Combustion analysis	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100005	20/11/2015 15:47:00	Opacity measurement	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100004	20/11/2015 15:47:00	Differential pressure	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100003	20/11/2015 15:47:00	Flue gas temperature	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100002	20/11/2015 15:47:00	Ambient temperature	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
15100000100001	20/11/2015 15:46:00	Ambient temperature	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
1501423100001	26/10/2015 17:05:00	Ambient temperature	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	Delete
	29/10/2015 08:00:00	Attestation SOLID	<input type="checkbox"/>	<input type="checkbox"/>	Delete
- Summary:** A section on the right showing summary information for the selected inspection.


Intervention type : Mesures GAZ
Date / Hour : 20/11/2015 16:08:00
- Preview:** A section on the right showing preview information for the selected inspection.

Start pressure : Measurement : 0 mbar
End pressure : Measurement : 0 mbar
Network airtightness : Measurement : 0 mbar : Conforme


- To delete an inspection from the complete database, click on the  button of the inspections list. A message is displayed to confirm deletion.
- Click on “OK” to confirm or “Cancel” to cancel the inspection deletion.

5.3.1. Database settings

- Click on “Database” menu then on “Database settings...”.
- The database configuration window opens.
- Click on the  button and define the save folder path.
- Select the recurrence, that is the automatic registration of the database:
 - Select the database registration frequency: from 1 to 30 hours or 1 to 30 days.
 - Or
 - Tick “When closing software” to save automatically the database when the software is closed.

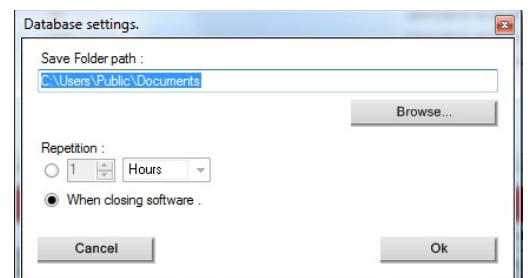

The screenshot shows the Database settings dialog box with the following fields and options:

- Save Folder path : 
- Repetition : 1 Hours
- When closing software .
- Buttons: Cancel, Ok

5.3.2. Save while using

To guarantee information saving, you shall regularly proceed this way:

- Click on “File” menu.
- Click on “Save database”.

5.3.3. Import a database

When opening LIGAZ-2 software, to recover a database:

- Click on “File” menu.
- Click on “Import database”.
- Go to the saving folder of the database, select the database to open then click on **OK**.

5.4. Edit an analysis report




From the complete database screen, it is possible to edit a measurements report.

- In the menu on the left of the screen, click on the required boiler for the report edition.
- Click on the **Measures** button.

The analysis report is displayed:

The screenshot shows a software window titled "KIGAZ-2 v. 1.9.812 - [New report.]". The interface includes a menu bar (File, Database, KIGAZ, Options, Windows, ?), a toolbar with navigation icons, and a status bar indicating "Analyzer connected". The main content area displays an "Analysis Report" form with the following sections:

- SPONSOR**: Includes fields for "caki" and "Address".
- Facility Address (IF DIFFERENT)**: Includes a "Boiler location" field.
- BOILER IDENTIFICATION**: Includes fields for "Brand", "Model" (value: b), "Energy" (value: Gaz Nat. Sahara/Fos), "Exhaust mode (AIR-TIGHT / NON AIR TIGHT)" (value: No Leakproof), "Serial number (IF AVAILABLE)", "Commissioning date", "Power rating" (value: 23 kW), "Last maintenance date (IF AVAILABLE)" (value: 20/11/2015), and "Last sweeping date (IF APPLICABLE AND AVAILABLE)".
- FORCED DRAUGHT BURNUER IDENTIFICATION (IF APPLICABLE)**: Includes fields for "Date", "Brand", and "Model".
- MEASUREMENT DEVICE USED**: Includes fields for "Brand" (value: KIMO) and "Reference" (value: KIGAZ 110).
- MEASUREMENTS DONE**: Includes fields for "Flue gas O₂", "Flue gas CO", "Flue gas CO₂", "Ambient temperature", "CO Max", "Ambient CO₂", "Internal temperature", and "Outgoing temperature".

- Use the  button to zoom in or zoom out on the report.
- Click on the  button to print the report or on the  button to export it in PDF format.



6. Set the analyser

LIGAZ-2 software allows to set the analyser. It is possible to:

- set the combustibles
- set the references (O₂ reference, altitude, atmospheric pressure)
- set the operators
- set date and time
- get details about sensors (State and serial number)
- set the header of printing
- see the battery level
- get information about the analyser, update it and send report to after-sales service


- Connect the analyser to the computer with the supplied USB cable.
- Connect the analyser on main power thanks to the supplied adapter to avoid extinguishing of the analyser (low battery).
- Click on “KIGAZ” in the menu bar.
- Go down to “Setting” then click on the parameter to modify.

Or

- Click on the  tool bar button or directly on the  button from the homepage.
“KIGAZ settings” window opens.




Changing parameters of the analyser has consequences on performed measurements and on the analysis calculation. Only a qualified technician is empowered to change the parameters of the device.

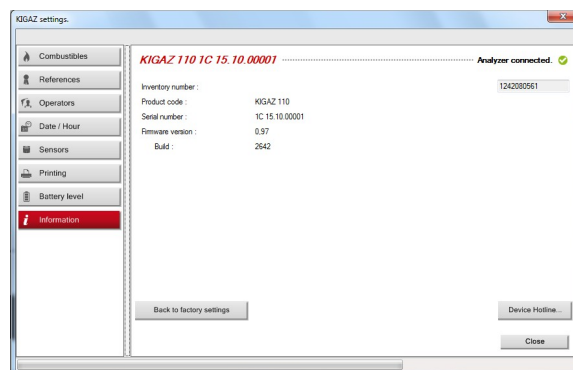

6.1. Change the combustibles


This window allows to change the list of combustibles programmed in the analyser. It also allows to modify features of each combustibles.


“KIGAZ settings” window is open on “Combustibles” or click on the  button.

- Click on the “Energy” field and select the combustible type: solid, liquid or gas.
- Double-click on one of the combustible features to modify.
- Enter the new value for the feature.
- Click on the  button to send modifications to the analyser.

6.2. Change the references

This window allows to modify the O₂ reference (percentage of oxygen in the air which the analyser is used), the altitude (altitude in which the analyser is used) and the atmospheric pressure (pressure in which the analyser is used).


“KIGAZ settings” window is open on “References” or click on the  button.

- Click on the field to modify.
- Write the new value.
- Click on the  button to send modifications to the analyser.

6.3. Manage the operators

This window allows to add, delete or modify an operator.


“KIGAZ settings” window is open on “Operators” or click on the  button.

- In the “Name” column, click on the field to write an operator name.
- Click on the  button to send modifications to the analyser.

6.4. Modify the date and time

This window allows to de sync the analyser time and the computer time.

“KIGAZ settings” window is open on “Date / Hour” or click on the  button.

- Click on the  button to adjust analyser time to computer time.

6.5. Sensors state

This window allows to access the sensors features of the connected analyser.


“KIGAZ settings” window is open on “Sensors” or click on the  button.

- The displayed features are:
 - Type of sensor (CO, NO,...)
 - State of sensor (connected, not connected...)
 - Serial number of the sensor

6.6. Set printings


This window allow to enter the 4 header lines of the ticket printed by the analyser.

“KIGAZ settings” window is open on “Printing” or click on the  button.

- Enter the required text in **“Header line 1, 2, 3 and 4”** lines.
- Click on the  button to send modifications to the analyser.

6.7. Battery level

This window allows to see the battery level of the analysis. The analyser must be turned on and on battery.

*“KIGAZ settings” window is open on “Battery level” or click on the  button.
The software displays the battery level.*

6.8. Access to information about the instrument and update the instrument

6.8.1. Access to information about the instrument

“KIGAZ settings” window is open on “Information” or click on the  button.

The following information is displayed:



- Product code: ex: KIGAZ 310
- Serial number: ex: 00.01.2057
- Firmware version: ex: 0.92
- Build: ex: 1247

It is possible to give an inventory number to the device (number selected and given by the user):



- Click on **“Inventory number”** field and enter the desired number.

6.8.2. Update the device

It is possible to update the firmware of the analyser, it means the internal software that allows to the analyser to work properly. It is also possible to install a 3rd language.

- Click on **KIGAZ** menu then go to **Settings** and click on **Information**, or click on the  tool bar button then on the  button.



The “KIGAZ settings” window is displayed.

- Click on the  button.
- The following window opens:*
- Click on the  button.

The connection parameters window opens:




Two choices are then possible:

- **The Internet connection is not protected by a proxy**

- Click on  button on the connection parameters window.
A progress bar is displayed then the available firmware number is displayed.
- Click on the  button.

The update lasts for a few minutes.

- Turn off then turn the device.
A black screen with a progress bar are displayed (see opposite) then It turns off itself.
- Turn on the device then go to **“Information”** menu of the analyser to check if the update has been taken into account.



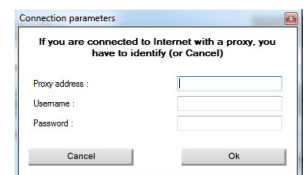
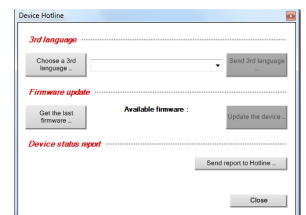


- **The Internet connection is protected by a proxy**

Address and serial number of the proxy, user name and corresponding password must be entered.



To get them into Windows 7:

- Click on **“Start”** (1) then on **“Control panel”** (2).
- In **“Control panel”** window, click on the up right on **“Large icons”** in **“View by”** (3).
- Click on **“Internet Options”** (4): the **“Internet Properties”** window opens.
- Click on **“Connections”** tab (5) then on **“LAN settings”** button (6): the **“Local Area Network (LAN) Settings”** window opens with the information about the proxy server (7).

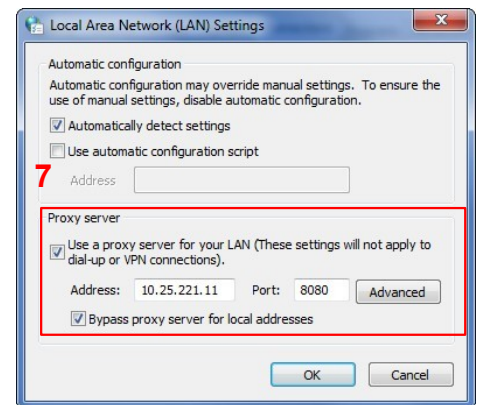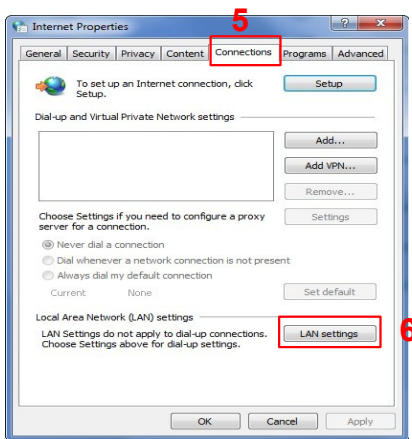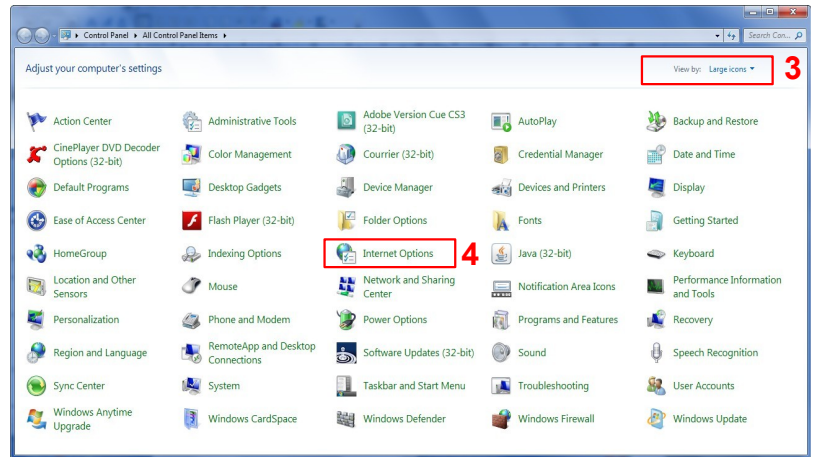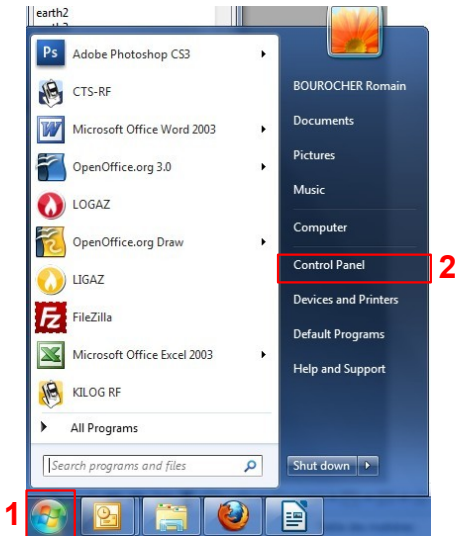

- Copy the address and the port in the **“Address”** line of the connection window as follows: 00.00.000.00:0000

Address Port


- Enter the user name and the corresponding password: data entered at the starting of the computer when the user logins.
- Click on the  button.
- Click on the  button.

The update lasts for a few minutes.


Turn off then turn on the device.

A black screen with a progress bar are displayed (see opposite) then the device turns off itself.

- Turn on the device then go to **“Information”** menu of the analyser to check if the update has been taken into account.



6.8.3. Install a 3rd language

- Select the language to send in the drop-down list box.
- Click on the  button.

6.8.4. Send a report of the device to the After-Sales Service

- Click on the button.
Kimo after-sales service will receive a report about the general state of the device only readable by the after-sales service.

6.8.5. Back to factory parameters

It is possible to set the device with the factory parameters.

The “Settings” window is open on “Information”.


- Click on the button.
The device is now set with the factory parameters.(see the factory parameters page 21).

7. Options

7.1. E-mail

This option allows to set the email sending parameters in order to send report to the after-sales service.

- Click on the “Options” menu then on the “Email” sub-menu.
The following window is displayed:
- Fill in the different fields:
 - **Email address of the outgoing mail:** e-mail address of the sender (p.durand@orange.fr)
 - **Outgoing mail server:** server address used to send e-mail (ex: smtp.orange.fr).
 - **Mail format:** plain text or html
 - **Advanced options:** by clicking on the button, the email setting window opens and allows to set the SMTP outgoing server. This information is delivered in the subscription documents of the Internet access provider
- Click on the button.

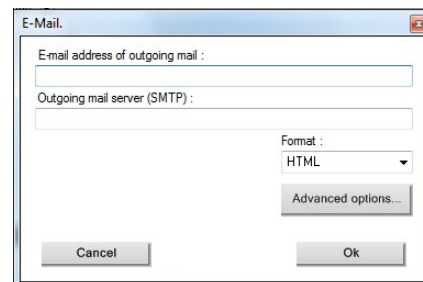

The screenshot shows a dialog box titled "E-Mail." with the following fields and controls:

- E-mail address of outgoing mail :
- Outgoing mail server (SMTP) :
- Format : (dropdown menu)
-
-
-

7.2. User information


This option allows to give information about the software user.

- Click on the “Options” menu then on the “User” sub-menu.
The following window is displayed:
- Fill in the different fields.
- Click on the button.

7.3. Change the language

This option allows to change the interface language.

- Click on “Options” menu.
- Click on “Languages” sub-menu.
- Select the required language.

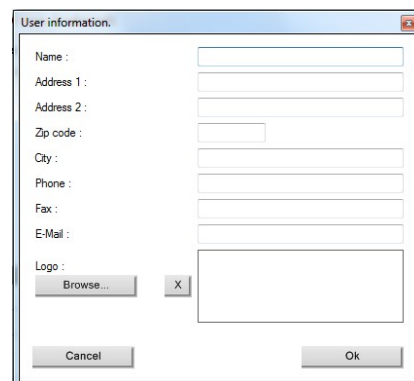

The screenshot shows a dialog box titled "User information." with the following fields and controls:


- Name :
- Address 1 :
- Address 2 :
- Zip code :
- City :
- Phone :
- Fax :
- E-Mail :
- Logo :
-
-

8. Customers / Boilers deletion of the analyser


It is possible to delete customers and/or boilers saved in the analyser via the LIGAZ-2 software.

- Connect the analyser to the computer then detect it with the LIGAZ-2 software.
- Click on “Menu” then “Customers/boilers deletion...”.


The following windows opens:

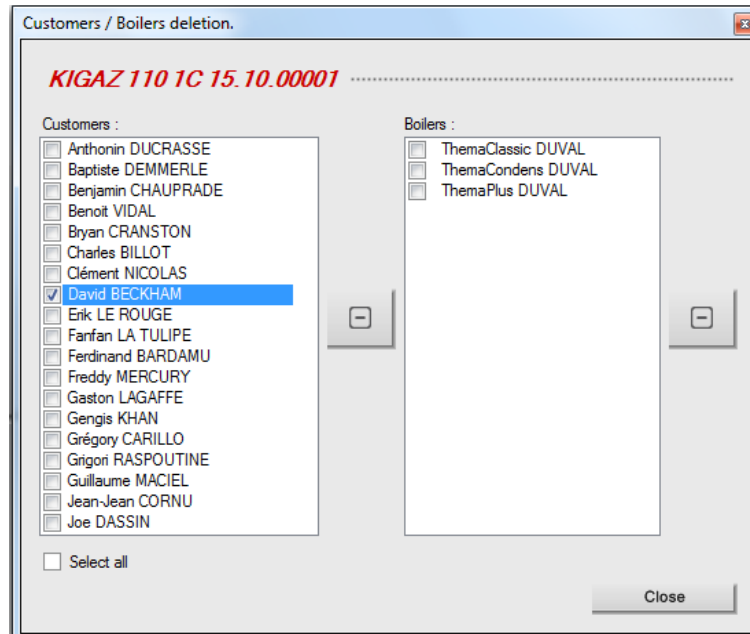

To delete a customer from the analyser:

- Tick the box of the customer to delete then click on the  button between “Customer” and “Boiler” columns.
A message of confirmation is displayed.
- Click on “Yes” to confirm the deletion.

To delete a boiler on the analyser:

- Click on the line of the customer to whom the boiler to delete is associated.
 - Tick the box of the boiler to delete then click on the  button on the left of the “Boilers” column.
A message of confirmation is displayed.
- Click on “Yes” to confirm the deletion.




Inspections linked to the deleted customer or boiler are also deleted.

9. Compare the instrument and software information

As we have seen, the LIGAZ-2 software allows to send information to the analyser or to delete information from the analyser:

- Sending customers or boilers to the **analyser**
- Download customers/boilers/inspections **from the KIGAZ to the software**
- Delete customers and boilers from the **analyser**

The **“Comparison of PC elements with KIGAZ”** function in the KIGAZ menu allows to update customers and boilers information in the analyser and in the LIGAZ-2 software databases. There are different possibilities.

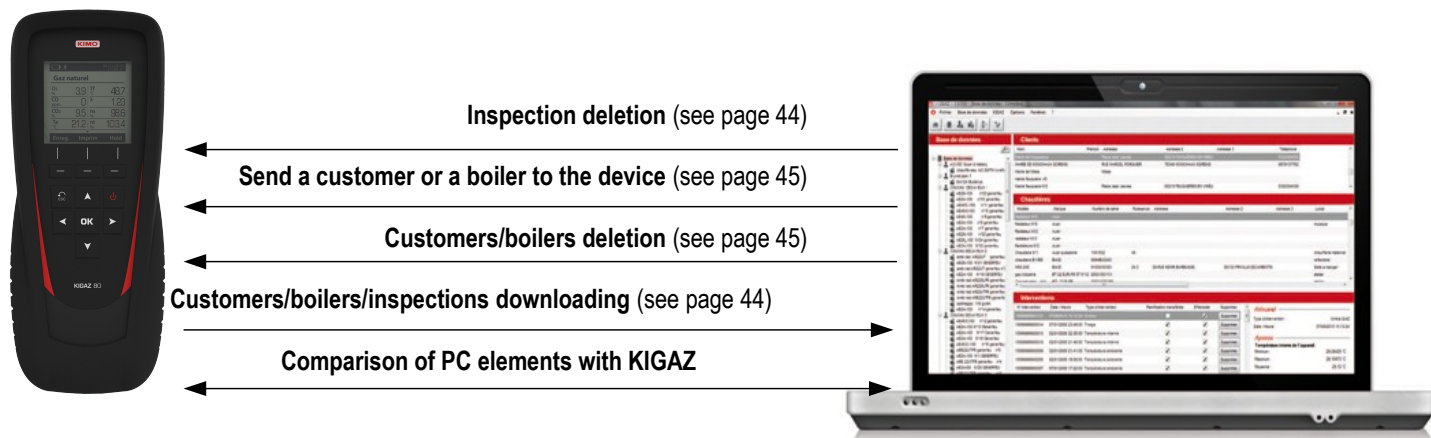

9.1. Add elements automatically in the databases

The LIGAZ-2 software will add automatically customers and boilers in the following cases:

- If the same customer is present in the analyser and the software **“Customers”** database but different boilers are associated to this customer, the software will add automatically the missing boilers in the **“Customers”** and **“Boilers”** databases.
- If a customer is present in the analyser with at least one associated boiler, the software will add it automatically in the **“Customers”** and **“Boilers”** databases. But if a customer is present in the analyser without associated boiler, the software will not add this customer in the **“Customers”** database.

Procedure:

- Click on **“KIGAZ”** menu.
- Click on **“Comparison of PC elements with KIGAZ”**.

9.2. Modification of customer and boilers features

The LIGAZ-2 software will compare the information: if a customer or a boiler is present in the analyser and the database but with different features, the software will ask which features have to be taken into account.

Procedure:

- Click on **“KIGAZ”**.
- Click on **“Comparison of PC elements with KIGAZ”**.

The following window opens:

Synchronization PC <-> KIGAZ.

Required synchronization:

Synchronize data of the PC and KIGAZ

Do nothing (keep the data as they are on the PC and KIGAZ)

Which data you want to keep?

PC data

KIGAZ data

BLANC ALAIN
Adresse : 12 RUE DU SOLEIL
LIEU DIT OUEST 24700 SAINT REMY SUR
Tel : 0553808500
E-Mail :

BLANC ALAIN
Adresse : RUE DU SOLEIL
LIEU DIT OUEST 24700 SAINT REMY SUR
Tel : 0553808500
E-Mail :

Apply this choice for other items to synchronize.

Ok

To keep the data as they are on the PC and KIGAZ:

- Tick the **“Do nothing (keep the data as they are on the PC and KIGAZ)”** box.
- Click on the **“OK”** button.

To update the information:

- Tick the **“Synchronise data of the PC and KIGAZ”** box.
- Tick the boxes of data to keep.
- Click on **“OK”** button.



To do the same actions on the following data, tick the **“Apply this choice for other items to synchronise”** box.



Once returned to KIMO, required waste collection will be assured in the respect of the environment in accordance to guidelines relating to WEEE.

www.kimo.fr

EXPORT DEPARTMENT
Boulevard de Beaubourg - Emerainville - BP 48
77312 MARNE LA VALLEE CEDEX 2
Tel : + 33.1.60.06.69.25 - Fax : + 33.1.60.06.69.29

