

It is recommended to replace the batteries immediately.

To replace the batteries unscrew the battery compartment cap and replace all four 1.5 V batteries while paying attention to their polarity. Make sure the gasket is in place before screwing back the cap.

Batteries should only be replaced in a non-hazardous area using the battery type specified in this instruction manual.

## ACCESSORIES

<b>MI59P</b>	Replaceable probe for <b>EC59 &amp; EC60</b>
<b>M10030B</b>	12.88 mS/cm calibration solution, 20 ml sachet, 25 pcs.
<b>M10031B</b>	1413 µS/cm calibration solution, 20 ml sachet, 25 pcs.
<b>MA9060</b>	12.88 mS/cm calibration solution, 230 ml bottle
<b>MA9061</b>	1413 µS/cm calibration solution, 230 ml bottle
<b>MA9016</b>	Cleaning solution, 230 ml
<b>M10000B</b>	Rinse solution, 20 ml sachet, 25 pcs.

## SPECIFICATIONS

### Range

0 to 3999 µS/cm / 0 to 2000 ppm (**EC59**)  
0.00 to 20.00 mS/cm / 0.00 to 10.00 ppt (**EC60**)  
0.0 to 60.0 °C / 32.0 to 140.0 °F

### Resolution

1 µS/cm / 1 ppm (**EC59**)  
0.01 mS/cm / 0.01 ppt (**EC60**)  
0.1 °C / 0.1 °F

### Accuracy (@25 °C / 77 °F)

±2 % FS (EC/TDS) / ±0.5 °C / ±1 °F

### Temperature Compensation

Automatic, with B=0.0 to 2.4 %/°C

<b>Calibration</b>	Automatic, 1 point
<b>Probe</b>	Replaceable <b>MI59P</b>
<b>Environment</b>	0 to 50 °C; 100 % RH max.
<b>Battery Type</b>	4 x 1.5 V; IEC LR44, A76
<b>Battery Life</b>	Approx. 100 hours of use
<b>Auto-off</b>	After 8 min. of non-use
<b>Dimensions / Weight</b>	200 x dia 38 mm / 100 g

## CERTIFICATION

Milwaukee Instruments conform to the CE European Directives.

**Disposal of Electrical & Electronic Equipment.** Do not treat this product as household waste. Hand it over to the appropriate collection point for the recycling of electrical and electronic equipment.

**Disposal of waste batteries.** This product contains batteries. Do not dispose of them with other household waste. Hand them over to the appropriate collection point for recycling.

Please note: proper product and battery disposal prevents potential negative consequences for human health and the environment. For detailed information, contact your local household waste disposal service or go to [www.milwaukeeinstruments.com](http://www.milwaukeeinstruments.com) (USA & CAN) or [www.milwaukeeinst.com](http://www.milwaukeeinst.com).

## RECOMMENDATION

Before using this product, make sure it is entirely suitable for your specific application and for the environment in which it is used. Any modification introduced by the user to the supplied equipment may compromise the tester's performance. For your and the tester's safety do not use or store the tester in hazardous environment. To avoid damage or burn, do not perform any measurement in microwave ovens.

## WARRANTY

These instruments are warranted against defects in materials and manufacturing for a period of 2 years from the date of purchase. Probe is warranted for 6 months. This warranty is limited to repair or free of charge replacement if the instrument cannot be repaired. Damage due to accidents, misuse, tampering or lack of prescribed maintenance is not covered by warranty. If service is required, contact your local Milwaukee Instruments Technical Service. If the repair is not covered by the warranty, you will be notified of the charges incurred. When shipping any instrument, make sure it is properly packaged for complete protection.



RoHS  
COMPLIANT



# USER MANUAL

## EC59 & EC60 PRO


### Waterproof 3-in-1 Low Range EC / TDS / Temperature Testers



[milwaukeeinstruments.com](http://milwaukeeinstruments.com) (USA & CAN)  
[milwaukeeinst.com](http://milwaukeeinst.com)

milwaukee



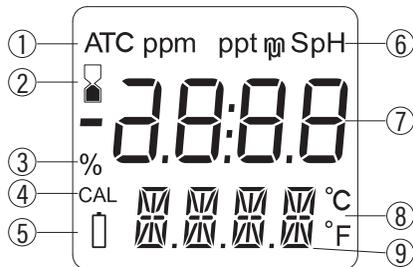

1. Automatic Temperature Compensation indicator
2. Instability indicator
3. Percent indicator
4. Calibration indicator
5. Low battery indicator
6. Measuring unit on main LCD
7. Main LCD
8. Temperature reading
9. Secondary LCD

## OPERATIONAL GUIDE

- Remove the probe cap and turn the tester on by pressing the ON/OFF/CAL button. All the used segments on the LCD will be visible for 1 second or as long as the button is pressed.
- Immerse the probe in the solution to be tested and select either EC or TDS mode with SET/HOLD.
- Stir gently and wait for the reading to stabilize, i.e. the hourglass symbol on the LCD turns off.
- The EC (or TDS) value is automatically compensated for temperature and will be displayed on the main LCD, while the temperature is shown on the secondary LCD.
- To freeze the display, while in measurement mode, press and hold the SET/HOLD button. The "HOLD" message appears on the secondary display and the reading will be frozen on the LCD. Press any button to return to normal mode.

- To turn the tester off, press the ON/OFF/CAL button. The "OFF" message will appear on the secondary display. Release the button.

### Notes:

*Before taking any measurement, make sure the tester is calibrated (the CAL tag is on). After use always turn the tester OFF, rinse the probe with water and store it with the protective cap.*

## SETUP

Setup mode allows the selection of temperature (°C or °F), TDS conversion factor (CONV) and temperature coefficient (BETA).

To enter the Setup mode, press the ON/OFF/CAL button until "CAL" on the secondary LCD is replaced by "TEMP" and the current temperature unit (e.g. TEMP °C). Then:

- for °C / °F selection: use the SET/HOLD button; then press the ON/OFF/CAL button three times to return to the normal measurement mode.
- to change the TDS factor value: after setting the temperature unit, press ON/OFF/CAL once to show the current value of the TDS conversion factor (e.g. 0.50 CONV). Select the desired value by using the SET/HOLD button, then press ON/OFF/CAL twice to return to the normal measurement mode.
- to change the temperature coefficient: after setting the TDS factor, press ON/OFF/CAL to show the current value of the temperature coefficient  $\beta$  (e.g. 2.1 BETA). Use the SET/HOLD button to set the desired value, then press ON/OFF/CAL to return to the normal measurement mode.

## CALIBRATION PROCEDURE

For better accuracy, frequent calibration of the tester is recommended. Calibration is also necessary after probe replacement, after testing aggressive chemicals and where extreme accuracy is required.

- From normal EC operation mode, press and hold the ON/OFF/CAL button until the

"OFF" message on the secondary LCD is substituted by "CAL". Release the button.

- Immerse the probe in the proper calibration solution: **M10030** (12.88 mS/cm) for **EC60** and **M10031** (1413  $\mu$ S/cm) for **EC59**.
- Once the calibration has been automatically performed, the LCD will show "OK" for 1 second and the tester will return to the normal measurement mode.
- Since there is a known relationship between EC and TDS readings, it is not necessary to calibrate the tester in TDS.

**Note:** *When the calibration procedure is completed, the CAL tag is turned on.*

- To exit calibration and return to the last calibration data press the SET/HOLD button. The secondary LCD displays "ESC" for 1 second and the tester returns to the normal measurement mode.
- To reset to the default values and clear a previous calibration, press the ON/OFF/CAL button after entering the calibration mode and before the calibration point is accepted. The secondary LCD displays "CLR" for 1 second, the tester resets to the default calibration and the CAL tag on the LCD turns off.

## PROBE REPLACEMENT

- Remove the protective cap and unscrew the plastic ring on the top of the probe.
- Pull out the **MI59P** probe and replace it with a new one.
- Make sure the gaskets are in place before screwing back the ring.

## BATTERY REPLACEMENT

When the batteries become weak, the battery symbol on the LCD will light up to advise that only a few hours of working time is remaining.

The tester is also provided with BEPS (Battery Error Prevention System), which avoids any erroneous readings due to low battery level by automatically switching the tester off.